



X'CAPE

Zippie® X'CAPE®



☐ with transit option

☐ without transit option

Supplier: This manual must be given to the user of this wheelchair.

Owner's Manual

Rider: Before using this wheelchair read this entire manual and save for future reference.

Zippie® X'CAPE®

☐ con opción de tránsito

☐ sin opción de tránsito

Manual de Instrucciones

Distribuidor: Este manual debe ser entregado al pasajero de esta silla de ruedas.

Pasajero: Antes de usar esta silla de ruedas, lea este manual en su totalidad y guárdelo para futura referencia.

Cada una de las sillas se envía con un manual de instrucciones en inglés. El manual en español o francés está disponible en formato PDF en nuestra página en Internet: www.SunriseMedical.com. Ingrese a la página del producto específico para descargar el manual, o comuníquese con el proveedor autorizado de Sunrise Medical.

Zippie® X'CAPE®

☐ avec option pour transport

☐ sans option pour transport

Manuel d'instructions

Fournisseur : Ce manuel doit être remis à l'utilisateur / utilisatrice de ce fauteuil roulant.

Utilisateur / Utilisatrice : Avant d'utiliser ce fauteuil roulant, lisez entièrement ce manuel et conservez-le pour le consulter ultérieurement.

Chaque fauteuil est livré avec un manuel d'instructions en anglais. Les versions en espagnol et en français sont à votre disposition en format PDF sur le site: www.SunriseMedical.com. Veuillez vous rendre à la page de votre produit pour télécharger le manuel dans la langue souhaitée, ou contactez un fournisseur agréé Sunrise Medical.



SUNRISE MEDICAL LISTENS

Thank you for choosing a Zippie wheelchair. We want to hear your questions or comments about this manual, the safety and reliability of your chair, and the service you receive from your Sunrise Medical dealer. Please feel free to write or call us at the address and telephone number below:

SUNRISE MEDICAL (US) LLC

Customer Service Department
12002 Volunteer Blvd.
Mount Juliet, TN 37122, USA
(800) 333-4000

Be sure to register your wheelchair and let us know if you change your address. This will allow us to keep you up to date with information about safety, new products, and options to increase your use and enjoyment of this wheelchair.

FOR ANSWERS TO YOUR QUESTIONS

Your authorized dealer knows your wheelchair best, and can answer most of your questions about chair safety, use and maintenance. For future reference, fill in the following:

Dealer: _____

Address: _____

Telephone: _____

Serial #: _____ Date/Purchased: _____

ADDITIONAL INFORMATION YOU SHOULD KNOW

No component of this chair was made with natural rubber latex.



DISPOSAL AND RECYCLING INFORMATION

When this product reaches the end of its life, please take it to an approved collection or recycling point designated by your local or state government. This wheelchair is manufactured using a variety of materials. Your product should not be disposed of as ordinary household waste. You should dispose of your wheelchair properly, according to local laws and regulations. Most materials that are used in the construction of this product are fully recyclable. The separate collection and recycling of your product at the time of disposal will help conserve natural resources and ensure that it is disposed in a manner that protects the environment.

Ensure you are the legal owner of the product prior to arranging for the product disposal in accordance with the above recommendations.

USER WARNING



WARNING

Attention wheelchair users, do not operate this wheelchair without first reading this owner's manual. If you do not understand the instructions and warnings of this owner's manual please contact your Authorized Dealer before operating this Zippie wheelchair. Failure to do so may result in damage and/or injury.

DEALER/TECHNICIAN WARNING




WARNING

Attention dealers and qualified technicians, do not operate or service this wheelchair without first reading this owner's manual. If you do not understand the instructions and warnings of this owner's manual please contact the Sunrise Medical technical service department before operating and/or servicing this Zippie wheelchair. Failure to do so may result in damage and/or injury.

I. INTRODUCTION	2	J. Rear wheels	13
II. TABLE OF CONTENTS	3	K. Rear wheel locks	13
III. YOUR DEVICE AND ITS PARTS	4	L. Modified seat systems	14
IV. NOTICE- READ BEFORE USE	4	M. Seat and back upholstery	14
A. Choose the right chair & safety options	4	N. Power drive	14
B. Review this manual often	4	O. Dynamic backrest	14
C. Warnings	4	P. Anti-tip receivers	14
V. GENERAL WARNINGS	5	VIII. USE AND MAINTENANCE	15
A. Weight limit	5	A. Introduction	15
B. Intended use	5	B. Critical safety checks	15
C. Attendants and caregivers	5	C. Cleaning tips	15
D. Accessories	5	D. Safety checklist	15
E. Know your chair	5	E. Troubleshooting chart	15
F. Reduce the risk of an accident	5	F. To mount & remove rear wheels	16
G. Safety checklist	5	G. Wheel locks	16
H. Changes and adjustments	5	H. Hub locks	16
I. Environmental conditions	6	I. Anti-tips	17
J. Terrain	6	J. Single post height adjustable armrest	17
K. Street use	6	K. Footrest system	18
L. Motor vehicle safety	6	L. Swing-away footrest	18
M. When you need help	7	M. Upholstered backrest	19
N. Choking hazard	7	N. Folding and unfolding	19
O. Pinch point	7	O. Integrated stroller handles	20
VI. SAFETY WARNINGS: FALLS & TIP-OVERS	8	P. Backrest	20
A. Center of balance	8	Q. Seat sling upholstery and cushion	20
B. Dressing or changing clothes	8	R. Storage tips	20
C. Obstacles	8	S. Inspect	20
D. Front caster lift	8	IX. DEALER SERVICE AND ADJUSTMENT	21
E. Reaching or leaning	8	A. Dealer service introduction	21
F. Moving backward	8	B. Critical maintenance tips	21
G. Escalators	9	C. Cleaning	21
H. Ramps, slopes and sidehills	9	D. Rear axles and axle plates	21
I. Transfers	10	E. Rear wheel axle nut adjustment	22
J. Curbs & single steps	10	F. Wheel locks	22
K. Climbing a curb or single step	11	G. Caster forks	23
L. Descending a curb or single step	11	H. Casters	23
M. Stairs	11	I. Anti-tip receivers	23
N. Climbing stairs	11	J. Armrest receiver attachment	24
O. Descending stairs	11	K. T-post armrest	24
VII. WARNINGS – COMPONENTS & OPTIONS	12	L. Standard flip-up armrest	24
A. Anti-tip tubes	12	M. Flip-up armrests (adjustable locking, and adjustable locking with adjustable length)	25
B. Armrests	12	N. Footrest system	25
C. Cushions & sling seats	12	O. Angle adjustable backrest	26
D. Fasteners	12	P. Xlock™ technology	27
E. Footrest	12	Q. Dynamic backrest	27
F. Pneumatic tires	12	R. Sideguard with t-post armrest	27
G. Positioning belts (optional)	13	S. Backrest tension adjustable	28
H. Push handles (optional)	13	X. SUNRISE LIMITED WARRANTY	29
I. Quick-release axles	13		

ZIPPIE X'CAPE®

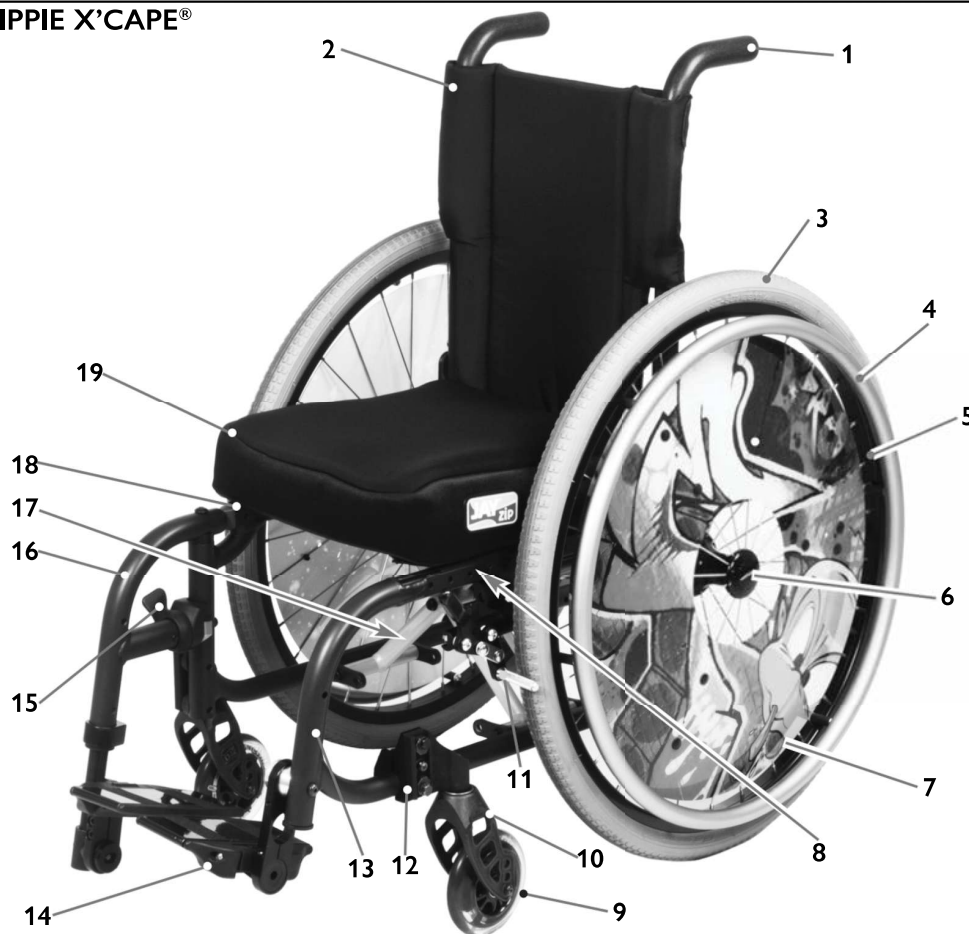

1. Push Handle/Backcane
2. Backrest
3. Pneumatic Tire
4. Aluminum Handrim
5. Aluminum Wheel Rim
6. Quick-Release Axle
7. Spoke cover
8. Versa Rail™ (Seat Rail)
9. Caster Wheel
10. Caster Fork
11. Wheel lock
12. Caster Clamp (Fixed)
13. Fixed Front Frame
14. Footrest System
15. Swing-Away latch release
16. Swing-Away Front Frame
17. XLOCK™ Crossbrace
18. Seat Sling
19. Cushion

NOTE – Not all options shown are available on the Fixed or Swing-away frame options of the Zippie X'CAPE®. Please refer to the order form for specific option availability.

IV. NOTICE - READ BEFORE USE

A. CHOOSE THE RIGHT CHAIR & SAFETY OPTIONS

Sunrise provides a choice of many wheelchair styles to meet your needs. This product is intended for single person use only. Final selection of the type of wheelchair, options and adjustments rests solely with you and your health care professional. Choosing the best chair for your unique mobility needs, will depend on such things as:

1. Your disability, strength, balance and coordination.
2. The types of hazards you must overcome in daily use (where you live and work, and other places you are likely to use your chair).
3. The need for options that will improve your positioning, safety and comfort (such as anti-tip tubes, positioning belts, or special seating systems).

B. REVIEW THIS MANUAL OFTEN

Before using this chair you, and each person who may assist you, should read this entire manual and make sure to follow all instructions. Review the warnings often, until they are second nature to you.

C. ⚠ WARNINGS

The word **“WARNING”** refers to a hazard or unsafe practice that may cause severe injury or death to you or to other persons. The “Warnings” are in three main sections, as follows:

1. V – GENERAL WARNINGS

Here you will find a safety checklist and a summary of risks you need to be aware of before you ride this chair.

2. VI – SAFETY WARNINGS: FALLS & TIP-OVERS

Here you will learn about practices for the safe use of your chair, and how to avoid a fall or tip-over while you perform daily activities in your chair.

3. VII – WARNINGS – COMPONENTS & OPTIONS

Here you will learn about the components of your chair and options you can select for safety. Consult your authorized **dealer** and your health care advisor to help you choose the best set-up and options for safe use.

NOTE – Where they apply, you will also find “Warnings” in other sections of this manual. Heed all warnings in these sections. If you fail to do so a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

A. WEIGHT LIMIT**WARNING**

NEVER exceed the weight limit specified by Sunrise Medical. The weight capacity provided by your manufacturer is for the combined weight of a rider and items carried using on-board storage. If you do exceed the weight limit, damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others. Never hang items greater than 5lbs (2.3kg) from stroller handle or seat back handle. A fall, tip-over, or loss of control may occur.

Weight Capacity:

Zippie X'CAPE® - 165 lbs / (75 kg)

B. INTENDED USE

The Zippie X'CAPE® wheelchair's intended use is to provide mobility to children limited to a sitting position.

**WARNING**

DO NOT use this device for purposes other than what is intended by the manufacturer.

1. The wheelchair is not designed for weight training and is unsafe for use as a seat while weight training. Weight training from the wheel-chair substantially changes the stability of the chair and may cause tipping.
2. DO NOT stand on the frame of the wheelchair.
3. NEVER allow someone to stand on your chair or use it as a step ladder.
4. This chair is designed for a single rider only.
5. Unauthorized modifications and use of parts or accessories not supplied or approved by Sunrise Medical may change the chair structure. This will void the warranty and may cause a safety hazard. If the warning is ignored, damage to your chair, and the potential severe injury of the person using the chair for unintended purposes can occur.

C. ATTENDANTS AND CAREGIVERS**WARNING**

Before you assist a rider, be sure to read all warnings contained in this manual and follow all instructions that apply. Be aware that after consulting a healthcare advisor, you will need to learn safe and proven body mechanics to use and create assistive methods best suited to your abilities.

D. ACCESSORIES**WARNING**

Unauthorized modifications or use of parts, or accessories not supplied or approved by Sunrise Medical may change the chair structure. This will void the warranty and may cause a safety hazard.

Some problems that may occur, but are not limited to:

1. Incorrect wheels and/or tires that put the rider at risk of a fall or tip-over.
2. Adding a component to the frame, changing the structural integrity of the chair.
3. Any modification or disassembly can potentially create an unsafe situation where rider and/or attendant are put at risk.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

E. KNOW YOUR CHAIR**WARNING**

Every wheelchair is different. Take the time to learn the feel of this chair before you begin riding. Start slowly, with easy, smooth strokes. If you are used to a different chair, you may use too much force and tip over. If you use too much force, damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

F. REDUCE THE RISK OF AN ACCIDENT**WARNING**

1. BEFORE you begin riding, you should be trained in the safe use of this chair by your health care advisor.
2. Practice bending, reaching and transfers until you know the limit of your ability. Have someone help you until you know what can cause a fall or tip-over and how to avoid doing so.
3. Be aware that you must develop your own methods for safe use best suited to your level of function and ability.
4. NEVER try a new maneuver on your own. Ask the advice of your health care provider to lower the risk of a fall or tip over.
5. Get to know the areas where you plan to use your chair. Look for hazards and learn how to avoid them.

G. SAFETY CHECKLIST**WARNING**

Before Each Use Of Your Chair:

1. Make sure the chair rolls easily and that all parts work smoothly. Check for noise, vibration, or a change in ease of use. (This may indicate low tire pressure, loose fasteners, or damage to your chair).
2. Inspect any problem. Your authorized dealer can help you find and correct the problem.
3. Check to see that both quick-release rear axles are locked. When locked, the axle button will "pop out" fully. If not locked, the wheel may come off and cause you to fall.
4. If your chair has anti-tip tubes, lock them in place.

H. CHANGES AND ADJUSTMENTS**WARNING**

1. If you modify or adjust this chair, it may increase the risk of a tip-over UNLESS you make other adjustments as well.
2. Consult your authorized dealer BEFORE you modify or adjust your chair.
3. We recommend that you use anti-tip tubes until you adapt to the change, and are sure you are not at risk to tip over.
4. Unauthorized modifications by the end-user, dealer or any other individual, including the use of parts not supplied or approved by Sunrise Medical may change the chair structure. This will void the warranty and may cause a safety hazard.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

I. ENVIRONMENTAL CONDITIONS

! WARNING

1. Use extra care if you must ride your chair on a wet or slick surface. If you are in doubt, ask for help.
2. Contact with water or excess moisture may cause your chair to rust or corrode. Avoid all extreme weather situations if possible.
 - a. Do not use your chair in a shower, pool, or other body of water. The chair tubing and parts are not water-tight and may rust or corrode from the inside.
 - b. Avoid excess moisture (for example, do not leave your chair in a damp bathroom while taking a shower).
 - c. Dry your chair as soon as you can if it gets wet or if you use water to clean it.
 - d. Avoid contact with salt or salty conditions as this may cause damage to the chair.



If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

J. TERRAIN

! WARNING

1. Based on ANSI/RESNA testing, Sunrise Medical recommends the use of a caster wheel with a minimum diameter of 5" if the wheelchair will be overcoming obstacles up to 1/2" on a regular basis.
2. Your chair is designed for use on firm, even surfaces such as concrete, asphalt, indoor flooring, and carpets.
3. Do not operate your chair in sand, loose soil, or over rocky terrain.
4. If you use your chair on terrain that is rougher than described above there is a danger that screws and bolts will loosen prematurely, and that damage to wheels or axles could put the rider at risk of a fall, tip-over, or loss of control.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

K. STREET USE

! WARNING

1. This product is not intended for street use.
2. Avoid streets whenever possible.
3. Obey and follow all legal pedestrian pathways, and laws that apply to pedestrians.
4. Be alert to the danger of motor vehicles in parking lots, or if you must cross a road.



If you fail to heed this warning, damage to your chair, and a possible collision may occur and cause severe injury to the rider or others.

L. MOTOR VEHICLE SAFETY 1 2

If possible and feasible, the rider should transfer to the Original Equipment Manufacturer (OEM) vehicle seat and use the OEM vehicle restraint.

Sunrise Medical does provide a WC-19 Wheelchair Tie-Down and Occupant Restraint System, otherwise called a Transit Option. To Identify whether your wheelchair has been manufactured with the Transit Option installed, look for four points of securement. Two Front points (A), and two rear points (B). These points are recognized by the securement point decal which can be found on or near the securement points.

If your wheelchair is equipped with the Transit Option, please review the Transit Securement supplement that was provided with the wheelchair for additional information and instructions. You can request a copy from your authorized dealer or call Sunrise medical at 1-800-333-4000 if you don't have it.

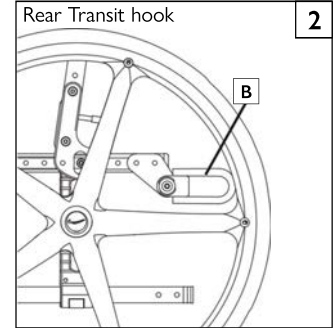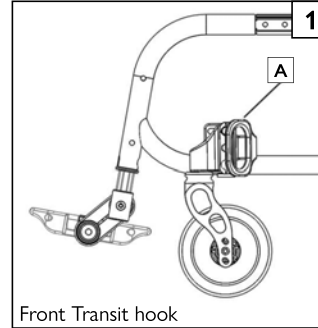

Look for this symbol on your wheelchair. It indicates wheelchair securement points which conform to ANSI/RESNA (1998) V.1 - Section 19 and/or ANSI/RESNA (2012) V.4 WC-19. For more Transit related information, see the "Transit Securement Supplement" included with your chair.

! WARNING

If your device is **NOT** equipped with the Transit Option:

1. NEVER let anyone sit in this chair while in a moving vehicle.
 - a. ALWAYS move the rider to an approved vehicle seat.
 - b. ALWAYS secure the rider with proper motor vehicle restraints.
2. In an accident or sudden stop the rider may be thrown from the chair. Wheelchair seat belts will not prevent this, and further injury may result from the belts or straps.
3. NEVER transport this chair in the front seat of a vehicle. It may shift and interfere with the driver.
4. ALWAYS secure this chair so that it cannot roll or shift.
5. DO NOT use any wheelchair that has been involved in a motor vehicle accident. A sudden stop and/or collision may structurally damage your wheelchair. There may have been a change to the structure of the chair, and/or damaged or broken some of the components. Wheelchairs involved in sudden stops should be inspected for possible failures in frame and/or components. Frame damage may be represented by but not limited to: visual cracks, dents, metal distortion, bends, or damage to the seating mounting. If the chair no longer drives straight, it could be damaged. If the wheelchair has been involved in an accident, discontinue use immediately and contact your Authorized Dealer for a thorough inspection. If damage is questionable or if there is concern regarding the condition of the chair, Sunrise Medical recommends replacement of the chair.
6. Wheelchairs involved in collisions should be replaced.

NOTE – The warranty is void on any wheelchair that is involved in a collision.

Failure to heed these warnings puts you and others that may assist you at a high risk of injury.

M. WHEN YOU NEED HELP**WARNING****For The Rider:**

Make sure that each person who helps you reads and follows all warnings and instructions that apply.

For Attendants:

1. Work with the rider's doctor, nurse or therapist to learn safe methods best suited to your abilities and those of the rider.
2. Tell the rider what you plan to do, and explain what you expect the rider to do. This will put the rider at ease and reduce the risk of an accident.
3. Make sure the chair has push handles. They provide secure points for you to hold the rear of the chair to prevent a fall or tip-over. Check to make sure push handle grips will not rotate or slip off.
4. To prevent injury to your back, use good posture and proper body mechanics. When you lift or support the rider or tilt the chair, bend your knees slightly and keep your back as upright and straight as you can.
5. Remind the rider to lean back when you tilt the chair backward.
6. When you descend a curb or single step, slowly lower the chair in one easy movement. Do not let the chair drop the last few inches to the ground. This may damage the chair or injure the rider.
7. To avoid tripping, unlock and rotate anti-tip tubes up, out of the way.
8. Whenever you aren't attending the wheelchair, ALWAYS use the wheellock to secure the rear wheels, and lock the anti-tip tubes in place.

If you fail to ask for help when in doubt, you run a high risk of a fall, tip-over or loss of control that may occur and cause severe injury to the rider or others.

N. CHOKING HAZARD**WARNING**

NOTE – Your chair consists of many small parts that could present a choking hazard to young children. Take care to put parts out of reach when doing any work on the chair.

O. PINCH POINT**WARNING**

NOTE – Your wheelchair has many moving parts that can create pinch points and possible finger traps. Be aware when making any adjustments, when folding and unfolding, when moving, and any other situation that could cause a pinch point situation.

A. CENTER OF BALANCE**WARNING**

The point where this chair will tip forward, back or to the side depends on its center of balance and stability. How your chair is set up, the options you select and the changes you make may affect the risk of a fall or tip-over.

1. The Most Important Adjustment Is:
The position of the rear wheels. The more you move the rear wheels forward, the more likely your chair will tip over backward.
2. The Center Of Balance Is Also Affected By:
 - a. A change in the set-up of your chair, including:
 - The distance between the rear wheels.
 - The amount of rear wheel camber.
 - The seat height and seat angle.
 - Backrest angle.
 - b. A change in your body position, posture or weight distribution.
 - c. Riding your chair on a ramp or slope.
 - d. A back pack or other options and the amount of added weight.
3. To Reduce The Risk Of An Accident:
 - a. Consult your doctor, nurse or therapist to find out what axle and caster position is best for you.
 - b. Consult your authorized dealer BEFORE you modify or adjust this chair. Be aware that you may need to make other changes to correct the center of balance.
 - c. Have someone help you until you know the balance points of your chair and how to avoid a tip-over.
 - d. Use anti-tip tubes.

If you fail to heed these warnings, you are at a high risk of a fall, tip-over or loss of control that could cause severe injury to the rider or others.

B. DRESSING OR CHANGING CLOTHES**WARNING**

Your weight may shift if you dress or change clothes while seated in this chair.

To reduce the risk of a fall or tip-over:

1. Rotate the front casters until they are as far forward as possible. This makes the chair more stable.
2. Lock anti-tip tubes in place. (If your chair does not have anti-tip tubes, back it up against a wall and lock both rear wheels).

If you fail to heed this warning, damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

C. OBSTACLES**WARNING**

Riding over curbs or obstacles can cause tipping and serious bodily harm. If you have any doubt that you can safely cross any curb or obstacle, ALWAYS ASK FOR HELP. Be aware of your riding skills and personal limitations. Develop new skills only with the help of a companion.

To avoid the risk of traversing obstacles:

1. Keep a lookout for danger – scan the area well ahead of your chair as you ride.
2. Make sure the floor areas where you live and work are level and free of obstructions.
3. Remove or cover threshold strips between rooms.
4. Install a ramp at entry or exit doors. Make sure there is not a drop off at the bottom of the ramp.
5. To Help Correct Your Center Of Balance:
 - a. Lean your upper body FORWARD slightly as you go UP over an obstacle.
 - b. Press your upper body BACKWARD as you go DOWN from a higher to a lower level.
6. If your chair has anti-tip tubes, do not go over an obstacle without help.

7. Keep both of your hands on the handrims as you go over an obstacle.
8. Never push or pull on an object (such as furniture or a doorjamb) to propel your chair.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

D. FRONT CASTER LIFT**WARNING**

Front caster lift can occur when the front wheels, ordinarily in contact with the ground, are either intentionally, or unintentionally caused to lift from the ground while the rear wheels remain in contact. Pitch control (partial or full) should NEVER be attempted without consulting your healthcare advisor and making sure that anti-tips are installed.

If you fail to heed this warning, you are at a high risk of damage to your chair, a fall, tip-over or loss of control that may occur and cause severe injury to the rider or others.

E. REACHING OR LEANING**WARNING**

If you reach or lean it will affect the center of balance of your chair. This may cause you to fall or tip over. When in doubt, ask for help or use a device to extend your reach.

1. NEVER reach or lean if you must shift your weight sideways or rise up off the seat.
2. NEVER reach or lean if you must move forward in your seat to do so. Always keep your buttocks in contact with the backrest.
3. NEVER reach with both hands (you may not be able to catch yourself to prevent a fall if the chair tips).
4. NEVER reach or lean to the rear unless your chair has anti-tip tubes locked in place.
5. DO NOT reach or lean over the top of the seat back. This may damage one or both backrest tubes and cause you to fall.
6. If You Must Reach Or Lean:
 - a. Do not lock the rear wheels. This creates a tip point and makes a fall or tip-over more likely.
 - b. Do not put pressure on the footrests.
 - c. Move your chair as close as you can to the object you wish to reach.
 - d. Do not try to pick up an object from the floor by reaching down between your knees. You are less likely to tip if you reach to the side of your chair.
 - e. Rotate the front casters until they are as far forward as possible. This makes the chair more stable.
 - f. Firmly grasp a rear wheel or an armrest with one hand. This will help to prevent a fall if the chair tips.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

F. MOVING BACKWARD**WARNING**

Use extra care when you move your chair backward. Your chair is most stable when you propel yourself forward. You may lose control or tip over if one of the rear wheels hits an object and stops rolling.

1. Propel your chair slowly and smoothly.
2. If your chair has anti-tip tubes, make sure to lock them in place.
3. Stop often and check to be sure your path is clear.

If you fail to heed this warning, you are at a high risk of damage to your chair, a fall, tip-over or loss of control that may occur and cause severe injury to the rider or others.

G. ESCALATORS**⚠ WARNING**

NEVER use this chair on an escalator, even with an attendant. If you do, a fall or tip-over is likely. *If you fail to heed this warning you and others that may be assisting you, are at a high risk of severe injury.*

H. RAMPS, SLOPES AND SIDEHILLS 3 4 5 6**⚠ WARNING**

Whenever possible, avoid riding on a slope, which includes a ramp or sidehill. This will change the center of balance of your chair. Your chair is less stable and more difficult to maneuver. when it is at an angle. When moving up a hill, anti-tip tubes may not prevent a fall or tip-over.

1. **DO NOT** use your chair on a slope steeper than 6°.
2. **ALWAYS** go as straight up and as straight down as you can. (Do not “cut the corner” on a slope or ramp).
3. **DO NOT** turn or change direction on a slope.
4. When you have to use a ramp, always stay in the **CENTER** of the ramp. Make sure ramp is wide enough that you have no risk of going off the edge.
5. **DO NOT** stop on a steep slope. If you stop, you may lose control of your chair.
6. **NEVER** use rear wheel locks to try to slow or stop your chair. This is likely to cause your chair to veer out of control.
7. **ALWAYS** be aware of:
 - a. Wet or slippery surfaces.
 - b. A change in grade on a slope (or a lip, bump, or depression). These may cause a fall or tip-over.
 - c. A drop-off at the bottom of a slope or ramp. A drop-off as small as 3/4 inch can stop a front caster and cause the chair to tip forward.
8. To Reduce The Risk Of A Fall Or Tip-Over:
 - a. Lean or press your body **UPHILL**. This will help adjust for the change in the center of balance caused by the slope or sidehill.
 - b. Keep pressure on the handrims to control your speed on a down slope. If you go too fast you may lose control.
 - c. **ASK FOR HELP** any time you are in doubt.
9. Ramps At Home & Work – For your safety, ramps at home and work must meet all legal requirements for your area:
 - a. **AVOID A DROP-OFF** – Make sure there is a section at the top or bottom to smooth out the transition.
 - b. **ALWAYS** stay in the center of the ramp and control your speed.


If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and can possibly cause severe injury to the rider or others.

For Attendants:

Follow these steps to help the rider go up or down a ramp:

1. Stay behind the chair.
2. Firmly grasp the handles.
3. For going up or down a ramp, the chair should always be facing forward.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

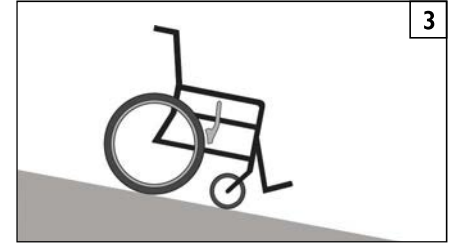


IF you need to go down a hill:

- a. The Downslope should be less than 6°.
- b. **GO SLOW** Control your speed.
- c. **ALWAYS** Go Straight down.
- d. **NEVER** turn on a hill.
- e. **ALWAYS** lean backward




IF you need to go up a hill:

- a. The Upslope should be less than 6°.
- b. **ALWAYS** Go Straight up.
- c. **NEVER** Stop on the upslope.
- d. **NEVER** turn on a hill.
- e. **ALWAYS** lean forward

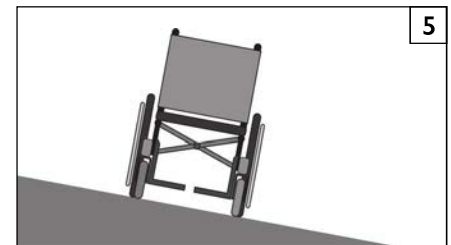

IF you need to traverse a Sidehill:

- a. The sidehill must be Less than 6° or you are at risk of a tip over.
- b. **DON'T STOP.**
- c. **DO NOT** make any turns on the sidehill.

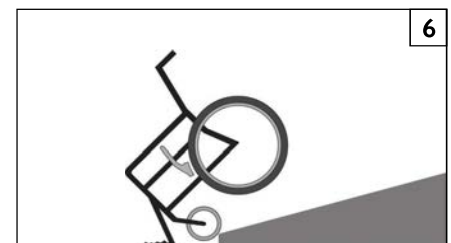

IF you need to traverse a Ramp:

- a. **Go slowly.**
- b. **Watch out for Drop-offs.**
- c. **ALWAYS** go straight up or straight down.
- d. **Stay centered on the Ramp.**

I. TRANSFERS 7 8**WARNING**

It is dangerous to transfer on your own. It requires good balance and agility. Be aware that there is a point during every transfer when the wheelchair seat is not below you. To avoid a fall:




1. Work with your health care advisor to learn safe methods for transfers.
 - a. Learn how to position your body and how to support yourself during a transfer.
 - b. Have someone help you until you learn safe transfer methods.
2. Lock the rear wheels before you transfer.
3. Be aware that the chair can still slide and/or tip. The wheel lock keeps the rear wheels from rolling while you are performing the transfer.
4. Make sure that the pneumatic tires are properly inflated. Low tire pressure may allow the rear wheel locks to slip. (see table in Section VII F "Pneumatic Tires" on page 12.
5. Move your chair as close as you can to the seat you are transferring to. If possible, use a transfer board.
6. Rotate the front casters until they are as far forward as possible.
7. If you can, remove the footrests, or swing them out of the way.
 - a. Make sure your feet do not catch in the space between the footrests.
 - b. Avoid putting weight on the footrests as this may cause the chair to tip.
8. Make sure armrests are removed, or out of the way, and do not interfere with the transfer.
9. Transfer as far back onto the seat surface as you can. This will reduce the risk that the chair will tip or move away from you.

Optimum transfer position



Before transferring:

1. **Flip-back or remove the armrests.**
2. **Swing-away or remove the footrests.**
3. **Make sure the wheel lock is set.**

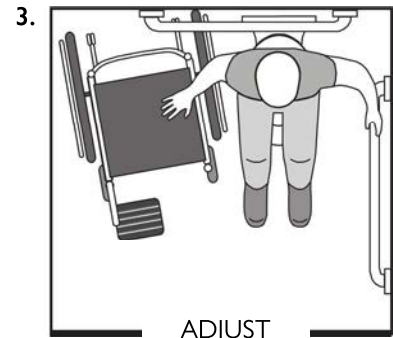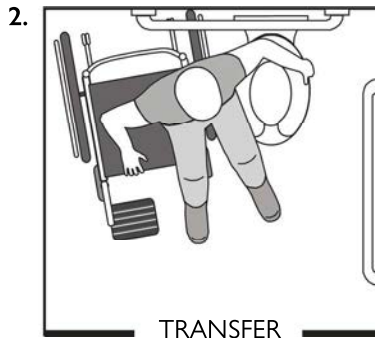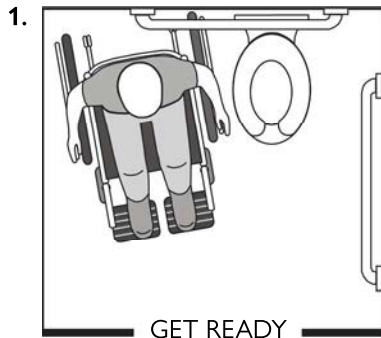**J. CURBS & SINGLE STEPS** 9**WARNING**

Before riding over curbs and negotiating even a single step, ALWAYS ask for assistance first. Curbs and steps can cause tipping and serious bodily harm. When in doubt as to your ability to avoid, or traverse any obstacle, always ask for help. Be aware of your riding skills and personal limitations. Develop new skills only with the help of a companion.

For Attendant: Each person who assists the rider with curbs and steps should read and follow all instructions and warnings pertaining to attendants, and caregivers.

1. Do not try to climb a high curb or step more than 4 inches (101 mm) high UNLESS you have help. Doing so may cause your chair to exceed its balance point and tip over.
2. Go straight up and straight down a curb or step. If you climb or descend at an angle, a fall or tip-over is likely.
3. Be aware that the impact of dropping down from a curb or step can damage your chair or loosen fasteners.


If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and can possibly cause severe injury to the rider or others.

K. CLIMBING A CURB OR SINGLE STEP 9**⚠ WARNING**

For Attendant: follow these steps to help the rider climb a curb or single step going BACKWARD:

1. Stay behind the chair.
2. Continue backward until the rear wheels contact the face of the curb or step. Lift and roll the rear wheels to the top of the curb.
3. Pull the chair backwards until the caster wheels have cleared the edge of the curb and return the chair to it's rolling position.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

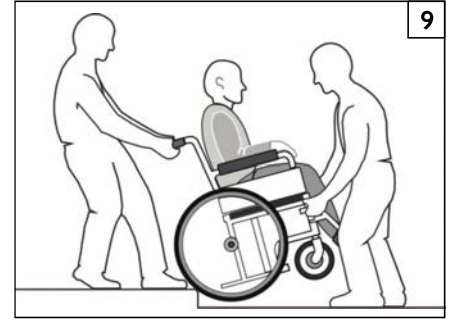**L. DESCENDING A CURB OR SINGLE STEP 9****⚠ WARNING**

For Attendant: Follow these steps to help a rider descend a curb or single step going FORWARD:


1. Stay at the rear of the chair.
2. Several feet before you reach the edge of the curb or step, tip the chair slightly and pull it backward.
3. When the chair is at it's balance point, carefully step forwards until the rear wheels reach the edge of the curb or step. Then allow the rear wheels to slowly roll down onto the lower level.
4. Push the chair forward until you are standing on the lower level.
5. When the rear wheels are safely on the lower level, tilt the chair back to its balance point.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

M. STAIRS 10**⚠ WARNING**

1. NEVER use this chair on stairs UNLESS you have someone to help you. Doing so is likely to cause a fall or tip-over.
2. Negotiating stairs with a wheelchair always requires at least 2 attendants for safety.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

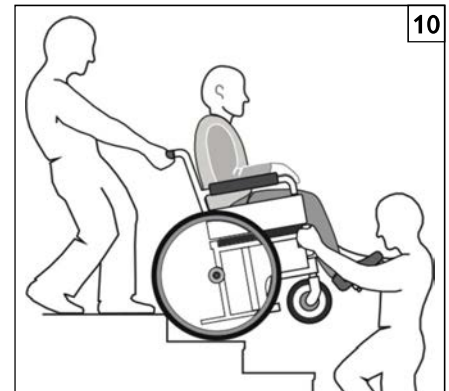**N. CLIMBING STAIRS 10****⚠ WARNING**

1. Use at least two attendants to move a chair and rider up stairs.
2. Move the chair and rider BACKWARD up the stairs.
3. The person at the rear is in control. He or she tilts the chair back to its balance point.
4. A second attendant at the front firmly grasps a non-detachable part of the front frame and lifts the chair up and over one stair at a time.
5. The attendants move to the next stair up. Repeat for each stair, until you reach the landing.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

O. DESCENDING STAIRS 10**⚠ WARNING**

1. Use at least two attendants to move a chair and rider down stairs.
2. Move the chair and rider FORWARD down the stairs.
3. The person at the rear is in control. He or she tilts the chair to the balance point of the rear wheels and rolls it to the edge of the top step.
4. A second attendant stands on the third step from the top and grasps the chair frame. He or she lowers the chair one step at a time by letting the rear wheels roll over the stair edge.
5. The attendants move to the next stair down. Repeat for each stair, until you reach the landing.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

A. ANTI-TIP TUBES**WARNING**

Anti-tip tubes can help keep your chair from tipping over backward in normal conditions.

1. Sunrise recommends the use of anti-tip tubes:
2. When locked in place (in the "down" position) anti-tip tubes should be BETWEEN 1-1/2 to 2 inches (38 to 51mm) off the ground.
 - a. If set **higher** than 2 inches (51mm), they may not prevent a tip-over
 - b. If set **lower** than 1-1/2 inches (38mm), they may "hang up" on obstacles and cause a fall or tip over.
3. If you have to climb or descend a curb, or overcome an obstacle it may be necessary to have an attendant make sure the anti-tip tubes are rotated up, and out of the way, so that the chair and rider do not get stuck and/or become unstable.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

B. ARMRESTS**WARNING**

Armrests detach and will not bear the weight of this chair.

1. NEVER lift this chair by its armrests. They may come loose or break.
2. Lift this chair only by non-detachable parts of the main frame.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

C. CUSHIONS & SLING SEATS**WARNING**

1. Zippie sling seats and standard foam cushions are not designed for the relief of pressure.
2. If you suffer from pressure sores or if you are at risk that they will occur, you may need a special seat system or a device to control your posture. Consult your doctor, nurse or therapist to find out if you need such a device for your well-being.
3. Seat slings are not intended to be used as a direct seating surface. A cushion or other seating surface should be placed on the sling before use.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

D. FASTENERS**WARNING**

Many of the screws, bolts and nuts on this chair are special high-strength fasteners. Use of improper fasteners may cause your chair to fail.

1. ONLY use fasteners provided by an authorized dealer (or ones of the same type and strength, as indicated by the markings on the heads).
2. Over- or under-tightened fasteners may fail or cause damage to chair parts.
3. If bolts or screws become loose, tighten them as soon as you can.

NOTE: For safety and performance it is best to not reuse fasteners.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

E. FOOTREST**WARNING**

1. At the lowest point, footrests should be AT LEAST 2 inches (51mm) off the ground. If set too LOW, they may "hang up" on obstacles you can expect to find in normal use. This may cause the chair to stop suddenly and tip forward.
2. To Avoid A Trip Or Fall When You Transfer:
 - a. Make sure your feet do not "hang up" or get caught in the space between the footrests.
 - b. Avoid putting weight on the footrests, as the chair may tip forward.
 - c. Footrests should be swung out of the way or removed whenever entering or exiting the wheelchair.
3. NEVER lift this chair by the footrests. Footrests detach and will not bear the weight of this chair. Lift this chair only by non-detachable parts of the main frame.
4. Never use the footrests of the chair to open doors, this may cause them to fail prematurely, and create an unsafe situation.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

F. PNEUMATIC TIRES**WARNING**

Proper inflation extends the life of your tires and makes your chair easier to use.

1. Do not use this chair if any of the tires are under- or over-inflated. Check weekly for proper inflation level, as listed on the tire sidewall.
2. Low pressure in a rear tire may cause the wheel lock on that side to slip and allow the wheel to turn when you do not expect it.
3. Low pressure in any of the tires may cause the chair to veer to one side and result in a loss of control.
4. Over-inflated tires may burst.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

Tires	X'CAPE	Recommended pressure or Pressure range	
		kPa	PSI
Pneumatic - 12"	X	270	40
Pneumatic - 16"	X	240	35
Pneumatic - 20"	X	448	65
Pneumatic - 22"	X	448	65
Pneumatic - 24"	X	517	75
Pneumatic - 26"	X	448	65
High pressure clincher (22")	X	690	100
High pressure clincher (24")	X	758	110
High pressure clincher (25")	X	758	110
Knobby V-Track (24")	X	448	65
Schwalbe Marathon (22")	X	586 - 1000	85 - 145
Schwalbe Marathon (24")	X	586 - 1000	85 - 145
Schwalbe speed	X	586 - 1000	85 - 145
Schwalbe Marathon plus Evol	X	586 - 1000	85 - 145

G. POSITIONING BELTS (OPTIONAL)

WARNING

The positioning belt is predominately used to support your posture. It can also be used to limit slipping and/or sliding that you might experience when the chair is in motion. The positioning belt is not a transit rated safety belt and should not be used in the place of a seat belt while being transported in a motor vehicle. Improper use of Positioning belts may cause severe injury or death. If you use a positioning belt, be sure to follow the recommendations in this section:

1. Make sure the rider does not slide down in the wheelchair seat. If this occurs, the rider may suffer chest compression or suffocate due to pressure from the belts.
2. The belts must be snug, but must not be so tight that they interfere with breathing. You should be able to slide your flat open hand between the belt and the rider.
3. A pelvic wedge or a similar device can help keep the rider from sliding down in the seat. Consult with the rider's doctor, nurse, or therapist to find out if the rider needs such a device.
4. Use positioning belts only with a rider who can cooperate. Make sure the rider can easily remove the belts in an emergency.
5. NEVER use positioning belts:
 - a. As a patient restraint. A restraint requires a doctor's order.
 - b. On a rider who is comatose or agitated.
 - c. As a motor vehicle restraint. In an accident or sudden stop the rider may be thrown from the chair. Wheelchair seat belts will not prevent this, and further injury may result from the belts or straps.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

H. PUSH HANDLES (OPTIONAL) 11

WARNING

When you have an attendant, make sure that this chair has push handles or stroller handles.

1. Push handles provide secure points for an attendant to hold the rear of this chair to prevent a fall or tip-over.
2. Check to make sure push handle grips will not rotate or slip off.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.



VII. WARNINGS – COMPONENTS & OPTIONS

I. QUICK-RELEASE AXLES

WARNING

1. Do not use this chair UNLESS you are sure that both quick-release rear axles are locked.
2. An axle is not locked until the quick-release button pops out fully.
3. An unlocked axle may come off during use, resulting in a fall, tip-over or loss of control and cause severe injury to the rider or others.
 - Quick-Release Axles should be periodically cleaned and inspected for function and signs of wear or bending. Replace as necessary.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

J. REAR WHEELS

WARNING

A change in set-up of the rear wheels will affect the center of balance of your chair.

1. The farther you move the rear axles FORWARD, the more likely it is that your chair will tip over backward.
2. Consult your healthcare advisor to find the best rear axle set-up for your chair. Do not change the set-up UNLESS you consult your health-care advisor first.
3. Adjust the rear wheel locks after you make any change to the rear axles.
 - a. If you fail to do so, the wheel locks may not work.
 - b. Make sure lock arms embed in the tires at least 1/8 inch (3.2mm) when locked.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

K. REAR WHEEL LOCKS

WARNING

Rear wheel locks are NOT designed to slow or stop a moving wheelchair. Use them only to keep the rear wheels from rolling when your chair is at a complete stop.

1. NEVER use rear wheel locks to try to slow or stop your chair when it is moving. Doing so may cause a fall or tip-over.
2. To keep the rear wheels from rolling, always set both rear wheel locks when you transfer to or from your chair.
3. Low pressure in a rear tire may cause the wheel lock on that side to slip and may allow the wheel to turn when you do not expect it.
4. Make sure lock arms embed in tires at least 1/8 inch (3.2mm) when locked. If you fail to do so, the locks may not work.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

L. MODIFIED SEAT SYSTEMS**WARNING**

Use of a seat system not approved by Sunrise may affect or interfere with other parts of the chair. This may cause the chair to tip over.

1. Do not change the seat system of your chair UNLESS you consult your authorized dealer first.
2. Use of a seating system not approved by Sunrise may affect or interfere with other parts of the chair.
3. Use of a seating system not provided by Sunrise is prohibited for transit use.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

M. SEAT AND BACK UPHOLSTERY**WARNING**

1. Replace worn or torn fabric of seat and seat back as soon as you can. If you fail to do so, the seat or seat back may fail.
2. Sling fabric will weaken with age and use. Look for fraying, thin spots, or stretching of fabrics especially at edges and seams.
3. "Dropping down" into your chair will weaken fabric and result in the need to inspect and replace the seat more often.
4. Be aware that laundering or excess moisture will reduce the flame retardation qualities of the fabric.
5. If Tension Adjustable upholstery is present, loosen straps or remove upholstery prior to folding or unfolding the chair.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

N. POWER DRIVE**WARNING**

Do not install a power drive on any Zippie Wheelchair that has not been approved by Sunrise Medical.

1. It will affect the center of balance of your chair and may cause a fall or tip-over.
2. It will alter the frame and void the warranty.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

VII. WARNINGS – COMPONENTS & OPTIONS**O. DYNAMIC BACKREST****WARNING**

Do not use any Dynamic Backrest setup other than what was provided by Sunrise Medical with your original chair.

1. It will affect the center of balance of your chair and may cause a fall or tip-over.
2. It will alter the frame and void the warranty.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

P. ANTI-TIP RECEIVERS**WARNING**

The Anti-tip receivers are designed to move with the axle location and are assembled in our manufacturing facilities.

1. Do not attempt to change the location of the anti-tip receivers, or remove them UNLESS you consult your authorized dealer first.
2. Use of an anti-tip system not approved by Sunrise may affect the center of gravity of the chair and lead to a fall or tip-over.

If you fail to heed these warnings damage to your chair, a fall, tip-over or loss of control may occur and cause severe injury to the rider or others.

**WARNING**

The owner of this chair is responsible for making sure that it has been setup and adjusted by a trained service professional under the advice of a healthcare advisor. The chair may require periodic safety checks or certain tool-free adjustments that may be performed by the owner, caregiver, or authorized dealer if desired. Always use parts and/or accessories that have been recommended or approved by Sunrise Medical when servicing this chair.

A. INTRODUCTION

1. Proper maintenance will improve performance and extend the useful life of your chair.
2. Clean your chair regularly. This will help you find loose or worn parts and make your chair easier to use. You will need a mild detergent solution and plenty of cleaning rags.
3. If discovered, repair or replace loose, worn, bent, or damaged parts **before using the chair**. ALWAYS be sure to use parts and/or accessories that have been recommended or approved by Sunrise Medical.
4. To protect your investment, have all major maintenance and repair work done by your authorized dealer.
5. **Inspect and maintain this chair strictly per the maintenance chart.**
6. **If you detect a problem, make sure to order parts, or have service, and repair work done at your authorized dealer before use.**
7. **At least once per year, have a complete inspection, safety check, and service of your chair made by an authorized dealer.**

B. CRITICAL SAFETY CHECKS

1. **Tire Air Pressure:**
Check air pressure in pneumatic tires at least **ONCE PER WEEK**. The wheel locks will not grip properly if you fail to maintain the air pressure shown on tire sidewall.
2. **Axles & Axle Sleeves:**
When checking axles and axle sleeves every six months, make sure they are clean and tight.
Loose sleeves will damage the axle plate and will affect performance.

C. CLEANING TIPS

1. **Paint Finish**
 - a. Clean the painted surfaces with mild soap or detergent at least once a month.
 - b. Protect the paint with a coat of non-abrasive auto wax every three months.
2. **Axles and Moving Parts**
 - a. Clean around axles and moving parts WEEKLY with a slightly damp (not wet) cloth.
 - b. Wipe off or blow away any fluff, dust or dirt on axles or moving parts.
3. **Upholstery**
 - a. Hand-wash (machine washing may damage fabric).
 - b. Drip-dry only. DO NOT machine dry as heat will damage fabric.
4. Basic Maintenance Materials available at local store
 - a. Tire Pump.
 - b. Tire Pressure Gauge
 - c. Clean rags or cotton cloth.
 - d. Teflon-based Lubricant.
 - e. Mild Detergent.

NOTE – You do not need to grease or oil the chair.

D. SAFETY CHECKLIST

Weekly	Monthly	3 Months	6 Months	Annually	Safety & Function Check
☒					Tire inflation level
☒					Wheel locks
		☒			Visually check for loose hardware
			☒		Armrests
			☒		Axle and axle sleeves
		☒			Quick-release axles
		☒			Wheels, tires and spokes
		☒			Casters
		☒			Anti-tip tubes
			☒		Frame, camber tubes, and crossbrace
	☒				Upholstery
				☒	Service by Authorized Dealer

NOTE – The user or caregiver should perform these weekly and monthly checks to maintain the safety of their chair. If an item is not working properly, please contact your authorized dealer.

E. TROUBLESHOOTING CHART

Symptom						Solution
Left turn in chair	Right turn in chair	Looseness in chair	Sluggish turning	Squeaks and rattles	Caster flutter	
☒	☒	☒	☒			Make sure tire pressure is correct and equal in both rear tires and front caster tires, if pneumatic.
		☒	☒	☒	☒	Make sure all nuts and bolts are tight.
		☒		☒		Make sure all spokes and nipples are tight on radial spoke wheels.
				☒		Use Tri-Flow Lubricant (Teflon®-based) between frame connections and parts.
☒	☒		☒		☒	Check for proper caster fork adjustment. See instructions for caster fork adjustment.

F. TO MOUNT & REMOVE REAR WHEELS 12 13**WARNING**

Do not use this chair UNLESS you are sure both quick-release axles are locked. An unlocked axle may come off during use and cause a fall.



1. To Install Wheel

- Depress quick-release button (A) fully. This will release tension on ball bearings at other end.
- Insert axle (B) through hub of rear wheel.
- Keep button (A) depressed as you slide axle (B) into axle sleeve (C).
- Release button to lock axle in axle sleeve. Adjust axle if it does not lock. See Section B.
- Repeat steps on other side.

NOTE – The axle is not locked until the quick-release button pops out fully (A). Check that the axle is locked by pulling on the wheel in the direction of the axle.

2. To Remove Wheel

- Depress quick-release button (A) fully.
- Remove wheel by sliding axle (B) completely out of axle sleeve (C).
- Repeat steps on other side.

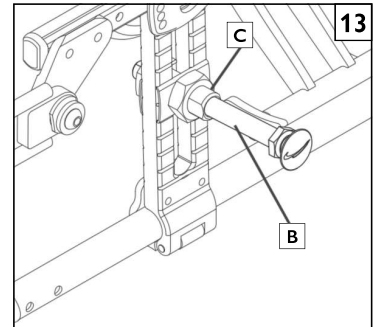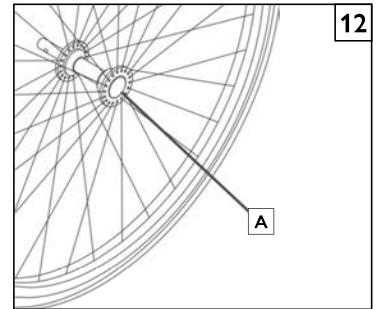
**G. WHEEL LOCKS** 14**WARNING**

Wheel locks are installed at Sunrise and should be adjusted by your qualified service person.

Inspect wheel locks weekly per the maintenance chart. Do not use your chair UNLESS you are sure both wheel locks can fully engage. A wheel lock that is not correctly adjusted may allow your chair to roll, or turn unexpectedly.

Wheel locks must be adjusted after making sure the tires have the correct air pressure. When fully engaged, the arm should be embedded into the tire at least 1/8" (3.2mm) to be effective.

If you find the wheel locks have slipped or are not working correctly contact your service provider for proper adjustment.

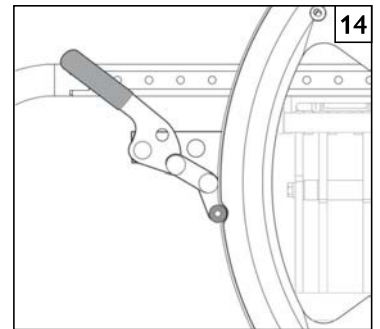**H. HUB LOCKS** 15 16**WARNING****To operate Hub Lock**

- To Lock rear wheels, press button (D). Lever (E) will flip outward.
- To unlock wheels, press Lever (E) back down until Button (D) pops back out. Each lever operates one side of the chair. To fully lock chair, both buttons must be pushed.



NOTE – Do not engage hub lock when chair is in motion.

To adjust the cables

- Loosen jam nut (F) using a 10mm wrench.
- Turn adjustment screw (G) in or out as necessary. Turning screw upward will loosen cable, turning downward will tighten cable.
- Re-tighten jam nut (F) against lever mount.
- Repeat steps 1-3 for opposite side of chair as necessary.

To adjust lever position

- Remove socket screw (H) and washer (I) from lever and backrest.
- Choose desired hole in backrest to mount lever and re-install screw and washer.
- Repeat steps 1-2 for opposite side of chair.

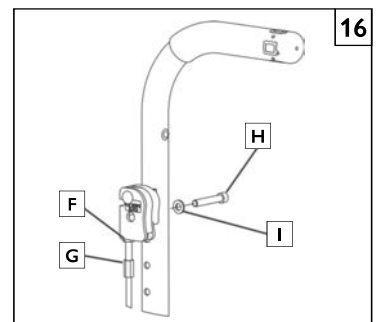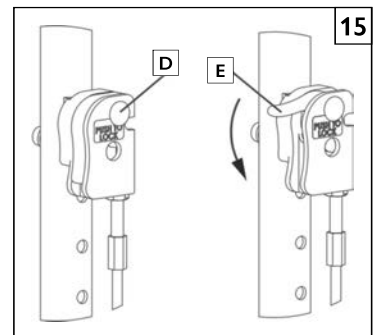


I. ANTI-TIPS 17 18 19

Sunrise Medical recommends anti-tip tubes for all wheelchairs.


1. Inserting Anti-Tip Tubes Into Receiver

- Press the rear anti-tip release pin (D) on the anti-tip tube so that both release pins are drawn inside.
- Insert into the anti-tip tube receiver (E).
- Turn the anti-tip tube down until release pin is positioned through the receiver mounting hole.
- Insert second anti-tip tube the same way.

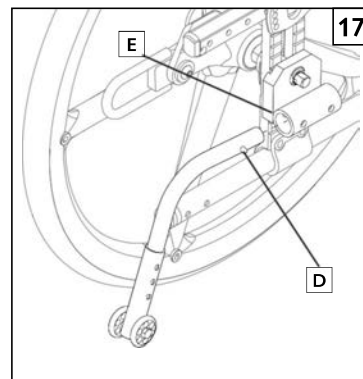**2. Adjusting Anti-Tip Tube Wheel**


The anti-tip tube wheels may have to be raised or lowered to achieve proper clearance 1-1/2" to 2" (38 to 51mm).

- Press the anti-tip wheel release pin (F) so that the release pin is drawn inside.
- Raise or lower to one of the three pre-drilled holes.
- Release pin.
- Adjust the second anti-tip tube wheel the same way. Both wheels should be at exactly the same height.

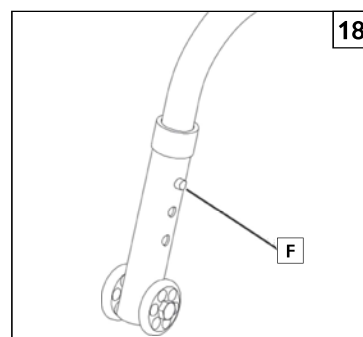**3. Turning Anti-Tip Tubes Up**

Turn anti-tip tubes up when being pushed by attendant, overcoming obstacles, or climbing curbs.

- Press the rear anti-tip tube release pin.
- Hold pin in and turn anti-tip tube up.
- Release pin, and make sure the anti-tip is locked in place.
- Repeat these steps with second anti-tip tube.

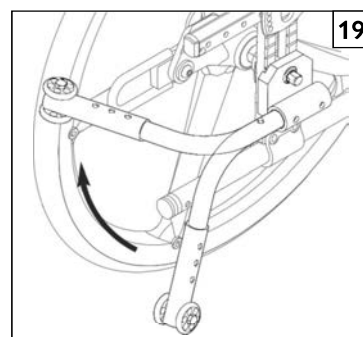**J. SINGLE POST HEIGHT ADJUSTABLE ARMREST** 20

Sunrise medical offers several different types of armrests. Fixed, swing-away, and flip-back armrests. Flip-back armrests can be detached or can flip back to allow lateral transfers. They are height adjustable (1" [25mm] increments) by flipping the adjustment lever and moving the armrest pad (1) up or down to the desired height.

1. Basic Installation

- Slide the outer armrest (4) into the receiver mounted to the wheelchair frame (7).
- The armrest should lock into place.

2. Height Adjustment


- Release the upper securing lever (2).
- Slide armpad up or down to desired height.
- Return lever to locked position.

3. Removing Armrest

- To remove, grasp the unlocking lever (3) and pull up on the armrest.

4. Replacing Armrest


- Slide armrest back into receiver.
- Make sure that the unlocking lever (3) returns to the locked position against armpost.

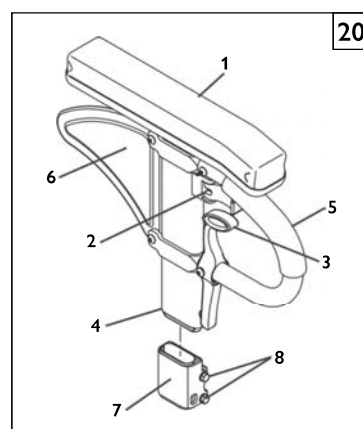

- Armrest pad
- Height Release Lever
- Release lever
- Outer armrest
- Transfer bar
- Side panel
- Receiver
- Receiver adjustment hardware

K. FOOTREST SYSTEM 21 22

Sunrise Medical offers either a single flip-up footplate (A), or dual footplates (B) that are able to accommodate all of the possible heights and adjustment angles that the rider may require for their comfort and support.

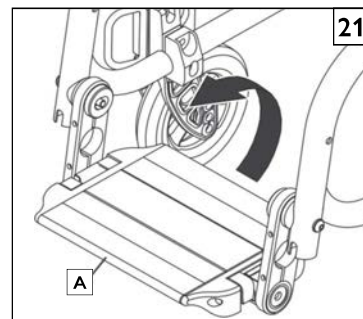**L. SWING-AWAY FOOTREST** 22 23

The footrest system can also accommodate a swing-away hanger (C) with dual footplates (B) that are both height adjustable and angle adjustable.



Swing-in-Swing-out Hangers and Footrests (80°, 90°)

1. Basic Footrest Installation

- From the side, place the pivot (C) into the top of the frame tube which guides the hanger into the correct alignment with the locking plate (D) on front frame tube.
- Rotate the footrest towards the front of the chair until it locks into place on locking plate.

2. Removal


- To remove footrest, release latch (E) by pulling lever upward or pushing lever downward.
- Rotate footrest inward or outward and lift.

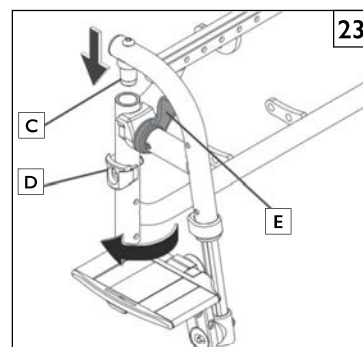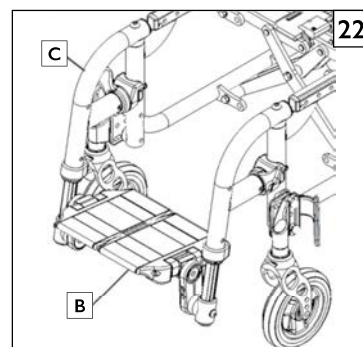**3. ELR Installation or Removal** 24

To install or remove Elevating Legrest (ELR) see instructions for Swing-away Footrest installation.

4. Elevation Adjustment

- To raise legrest, lift to desired position. Legrest will automatically lock in place.
- To lower legrest, while seated in chair, press release lever (D) down and lower legrest to desired position. Legrest will automatically lock in place.

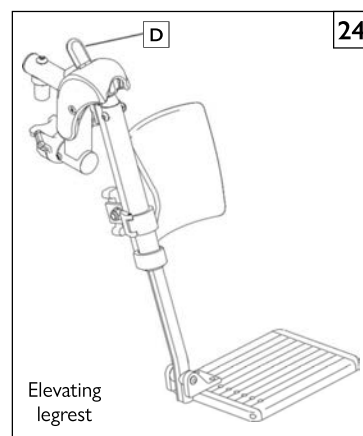

M. UPHOLSTERED BACKREST 25**1. Locking the upholstered Backrest into place**

Zippie wheelchairs with depth adjustable backs are shipped with the backrest/stroller handles (F) in a folded position. To secure backrest/stroller handles, lift backrest/stroller handles to upright position. When secured, backrest release pin (H) will lock into place.

2. Adding or Removing upholstered Backrest

- Check monthly for excessive stretching of the upholstery, or loose attaching hardware. If you determine the upholstery is no longer tight, contact your service representative for a replacement.
- If you need to replace the backrest upholstery, or remove it to add a solid backrest, start by removing the upholstery securing screw (G) from both backrests, and pull the upholstery off of the backposts.


**N. FOLDING AND UNFOLDING** 26 27 28**WARNING**

Possible pinch point! BE CAREFUL.

- If seat sling is not present during folding or unfolding, use the "Push to lock Tab" to open the chair.
- Use flat palms to depress the chair when opening.

1. Folding the Wheelchair


- Remove quick-release wheels (optional).
 - Depress quick-release button on the axle.
 - Remove wheel by sliding out quick-release axle from axle bracket.
 - Repeat with the other wheel.
- Flip up the footrests to a vertical position before folding the wheelchair.
- Grasp the seat sling folding strap (A) and lift up sharply until the wheelchair is folded.

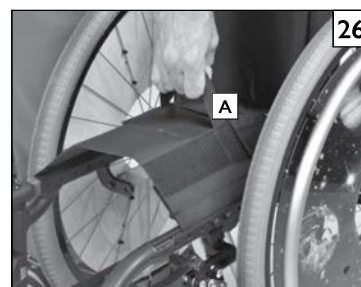**2. Unfolding the Wheelchair**

- Replace quick-release wheel (optional) by depressing the quick-release button on the axle.
- Slide it into the axle sleeve until it locks.
- Repeat with other wheel.
- Tilt the wheelchair toward you far enough to take the weight off the opposite wheel.
- Push down on the center of the seat sling, elastic window, and locking tab (B) until the wheelchair is completely opened.




NOTE – Ensure that footrests are flipped down, and locked prior to use.

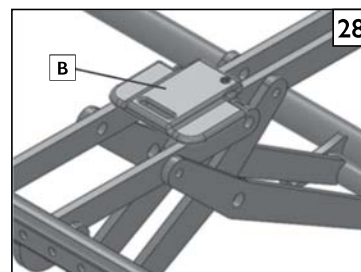

O. INTEGRATED STROLLER HANDLES 29**1. Positioning Swing-Away Adjustable Stroller Handles (option)**

Loosen push handle (C) by pushing the black button (D). You can then raise or lower the stroller handle to the desired position.

NOTE – For easy storage and portability, push handles will swing in and stroller handles fold flat.

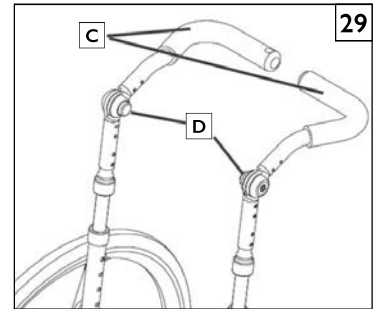
**P. BACKREST** 30**1. Folding the backrest**

- For easier storage and transport, Locate the backrest release pin lever (E) on both sides and pull up on the levers while pushing the backrest forward.

2. Unfolding the backrest

- To secure the back rest in a riding position, lift by the handles to an upright position. When secured, the backrest release pin will lock into place.

NOTE – For easy storage and portability, push handles should fold flat and not interfere with folding.

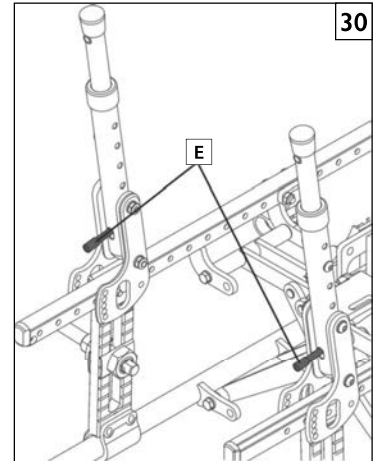**Q. SEAT SLING UPHOLSTERY AND CUSHION** 31

The seat sling can be adjusted through the use of hook and loop material beneath the seat. The seat sling also includes a folding strap on the seat to assist in folding the chair.

NOTE – The seat sling folding strap is not intended as a carrying strap.

1. Adjustment

- Remove seat rail end caps at the front or rear of the chair (D).
- Slide the seat sling, plastic retaining rods, and spacers (if present) from the channels in the seat rails.
- For fixed front frame, You must remove the 4 screws (E) that hold the rear caps and remove the caps. By removing the retaining rods first you can then remove the sling upholstery.
- Readjust hook and loop material to obtain the desired tension in the seat sling.
- Reinsert the seat sling and plastic retaining rods into the channels in the seat rails.

NOTE – The seat sling needs to be installed so that the “window” (F) is aligned with the locking tab.


- Replace the end caps.

2. Seat sling Upholstery

- Check monthly for excessive stretching of the upholstery or loose attaching hardware. If you determine the upholstery can no longer be adjusted tight, contact your service representative for a replacement.

3. Cushion Installation

- Place cushion on the seat sling with hook material side down. The beveled edge of the cushion should be facing toward the front of your chair.
- Press firmly into place.

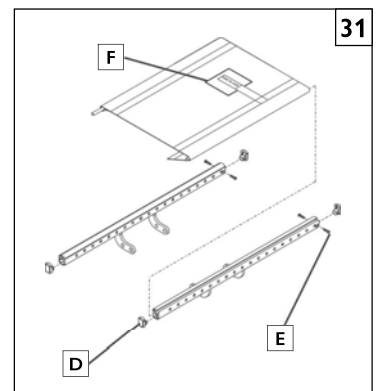**R. STORAGE TIPS**

- Store your chair in a clean, dry area. If you fail to do so, parts may rust or corrode.
- Before using your chair, make sure it is in proper working order. Inspect and service all items on the “Maintenance Chart”.
- If stored for more than three months, have your chair inspected by an authorized dealer before use.

S. INSPECT

After the wheelchair is assembled and adjusted, it should roll smoothly and easily. All accessories should also perform smoothly. If you have any problems, follow these procedures:

- Review the set-up and check-out sections and operating guide to make sure chair was properly prepared.**
- Review troubleshooting guide.**
- If your problem persists, contact your authorized dealer. If you still have a problem after contacting your authorized dealer, contact Sunrise Medical customer service. See the introduction page for details on how to contact your authorized dealer or Sunrise Medical customer service.**

⚠ WARNING

The owner of this chair is responsible for making sure that it has been setup and adjusted by a trained service professional under the advice of a healthcare advisor. Service and/or adjustments should only be done with the advice of a healthcare professional. Always use parts and/or accessories that have been recommended and approved by Sunrise Medical when servicing this chair.

A. DEALER SERVICE INTRODUCTION

1. At least once per year, this chair should have a complete inspection, safety check, and regular service made by an authorized dealer.
2. Torque settings— A torque setting is the optimum tightening which should be made on a particular fastener. It is important to use proper torque settings where specified.
3. If you have discovered a worn, bent, or damaged part, repair or replace them with recommended parts **before returning this chair to service.**
4. All major maintenance and repair work should be done by the authorized dealer.

B. CRITICAL MAINTENANCE TIPS

1. Torque settings:

A torque setting is the optimum tightening which should be made on a particular fastener. It is important to use proper torque settings where specified. When not specified, torque settings should be: M5 fasteners = 44 in-lbs (5 Nm), M6 fasteners = 62 in-lbs (7 Nm), M8 fasteners = 88 in-lbs (10 Nm). For all others torque setting should be 60 in-lbs (6.8 Nm). All joints secured with threaded fasteners will relax over time resulting in an actual torque that is lower than the initial torque setting. This is especially applicable for joints with elastic components.

2. Dealer Service and Adjustment Reference materials:

Go to www.sunrisemedical.com for parts manuals, instruction sheets, and instructional videos that will aid in the repair of the Zippie Family of wheelchairs.

C. CLEANING

1. Paint Finish

- a. Clean the painted surfaces with mild soap or detergent.
- b. Protect the paint with a coat of non-abrasive auto wax.

2. Axles and Moving Parts

- a. Clean around axles and moving parts with a slightly damp (not wet) cloth.
- b. Wipe off or blow away any fluff, dust or dirt on axles or moving parts.
- c. DO NOT USE 3 in 1 oil, or WD-40 ® for lubrication. Only use Teflon based lubricant when working on this wheelchair.

D. REAR AXLES AND AXLE PLATES 32 33

The most important adjustment on the Zippie wheelchair is the position of the rear axle. The center of gravity, wheel camber, and wheelbase are all determined by the axle adjustment.

Use a torque setting of 360 in-lbs (40.7Nm). when adjusting rear axle.

⚠ WARNING

The more you move the rear wheels forward, the more likely the chair will tip over backwards. Always make adjustments in small increments, and check the stability of the chair with a spotter to prevent a tip-over. Sunrise Medical recommends that anti-tip tubes are always used in conjunction with this type of adjustment.

1. Center of Gravity

Moving the center of gravity to the front will lighten the force required to turn the chair. The further back the axle, the more stable the chair becomes. The center of gravity is adjusted by moving indexed axle plate (A) forward or backward on the Zippie Frame (B). Moving the axle forward will increase your turning speed and lighten the front end.



- a. Loosen all hardware (C,D,E,F) on both sides of the chair and move the axle/backrest assembly to the correct position.
- b. Make sure that the ridges in indexing washer (D) are fully engaged before tightening axle nut.
- c. Tighten Screws (E) to 65 in-lbs (7.3Nm), and (F) to 120 in-lbs (13.6Nm).

NOTE – Adjustment holes in the versa rail provide 1" (25mm) Center of Gravity adjustments. Switching axle plates from side to side allows 1/2" (12.7mm) adjustments.



TOOLS YOU WILL NEED

1. Imperial Hex key set
2. Metric Hex key set
3. Imperial Open-end Wrench set
4. Metric Open-end Wrench set
5. Torque wrench
6. Imperial Hex bit Socket set
7. Metric Hex bit Socket set
8. Phillips and Flat screwdrivers

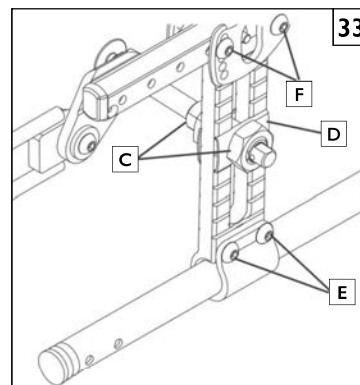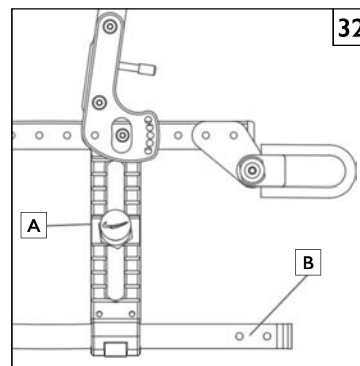

2. Wheel Camber 34

The wheel camber adjustment provides greater side-to-side stability due to the increased width and angle of the wheelbase. The wheel camber adjustment also allows for quicker turning and greater access to the top of the handrims.

Wheel camber is preset at the factory at 3°. You can achieve a 0° camber by removing the axle sleeve (A) and camber washers (D) and flipping them 180°.

NOTE – Adjusting your chair's center of gravity will require re-adjusting the location of the wheel locks (if provided). See Section G for instructions on adjusting the wheel locks.

3. Wheel Base Width Adjustment 34

Adjusting the wheelbase width allows the rider the option to move the wheels closer or further away from the hips. It also compensates for camber adjustment and gives the proper wheel spacing to maximize pushing efficiency.

- Loosen the nuts and reposition the axle sleeve (A) to the desired width.
- Retighten nuts to a torque of 360 in-lbs (40.1Nm).

4. Seat Height Adjustment 35

Seat height can be adjusted by loosening the large axle sleeve nuts (B), enough so that the axle washers will move along the axle plate vertically in the slots. Be sure to adjust both sides of the chair to an equal vertical seat height adjustment.

NOTE – Be sure the ridges for indexing washers are fully engaged in axle plate grooves before tightening.

NOTE – A front caster adjustment should be made to correspond with any change in seat height.

NOTE – In most cases the Anti-tip Receiver is used as the internal axle nut in this assembly. Loosen the external axle sleeve nut enough so that the whole assembly can be adjusted up or down. Tighten the axle sleeve nut to 360 in-lbs (40.1Nm) when the adjustment is complete.

E. REAR WHEEL AXLE NUT ADJUSTMENT 36

Tight axle sleeves should be maintained for proper performance of the wheelchair.

- To adjust the axle (C) you will need a 3/4" wrench to turn the outside axle nuts (E).
- You will also need a 1/2" wrench to lodge the ball bearings (D), on the opposite end of the axle, and prevent the axle from turning.
- Turn the outside axle nut (F) clockwise to tighten.
- There should only be zero to ten thousandths of an inch (.010" (.254mm)) of play.

F. WHEEL LOCKS 37 38

This Zippie chair is shipped with one of three types of wheel locks. Wheel locks are installed at the factory unless requested otherwise.

Use a torque setting of 120 in-lbs (13.6Nm). If setting up the wheel locks for your customer.

1. High-Mount Push-to-Lock or Pull-to-Lock Wheel Locks Adjustment.

- Using a 3/16 inch hex key, loosen the clamp screw (G) in the clamp.
- Slide the wheel lock toward the rear wheel until the wheel lock is embedded into the tire to prevent wheel movement, when in the locked position.
- You can also adjust the wheel lock angle by rotating the clamp while it is loose.
- Tighten screw to 120 in-lbs (13.6Nm).






2. Ergo Scissor Wheel Locks or Compact Wheel Locks.

Loosen the screws (G) on the top of each clamp using a 3/16 inch hex key. Slide assembly toward rear wheel until clamp embeds into tire to prevent wheel movement when in locked position. Adjust angle position. Tighten screws to 120 in-lbs (13.6Nm).

NOTE – Clamp and wheel lock may need to be rotated to clear frame tubing.

3. Foot Lock.


The foot lock should be kept at the factory settings, it will generally not need any adjustment to keep it functioning.

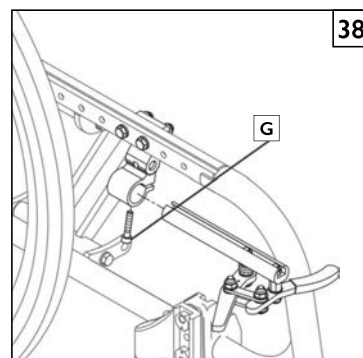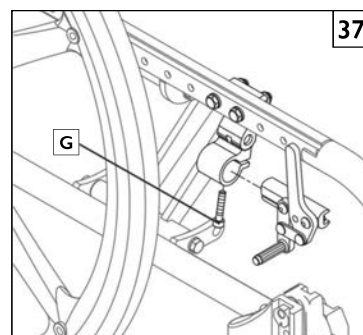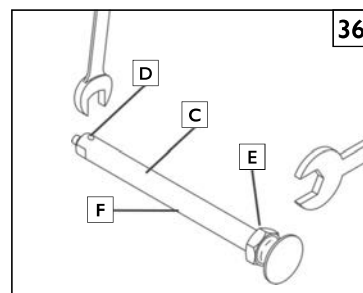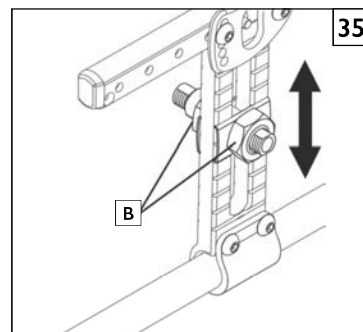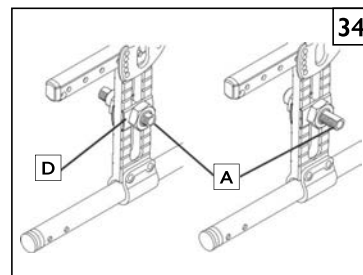

G. CASTER FORKS 39

Three-hole caster forks allow the interchanging of some caster wheels and height adjustment when adjusting seat height. To adjust, loosen the bolt and remove the caster wheel. Change the caster size and/or position of the caster upward or downward in pre-drilled holes (1/2" inch (12.7mm) apart) on caster fork. Replace bolt and tighten securely.

Use a torque setting of 40 in-lbs (4.5Nm) when adjusting the caster forks.

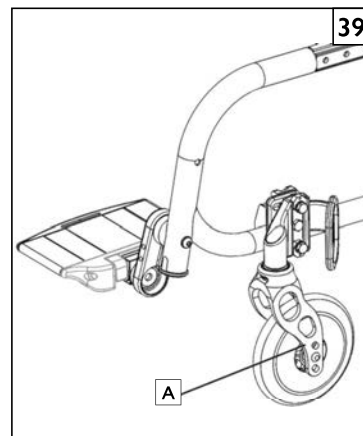
**H. CASTERS** 40

Use a torque setting of 144 in-lbs (16.3Nm) when adjusting the casters.

1. Caster Angle Adjustment

For optimum performance, and after a seat height adjustment, the caster housing should always be at a 90° angle to the floor (perpendicular to the ground). This adjustment is made with an eccentric (offset) washer and hardware.


- To change the angle, place the chair on a flat surface (such as a table).
- Remove the nuts and washers (B) from the back side of the caster plate. The caster plate is slotted at the top and bottom for adjustment.
- Place a large right triangle against the table surface and the front surface of the caster bearing housing.
- This will align the caster stem rotational axis perpendicular to the floor surface.
- Rotate the eccentric washers (C) independently until they fall into position.
- When the alignment is correct, re-tighten the hardware.
- Repeat the process for the other caster.

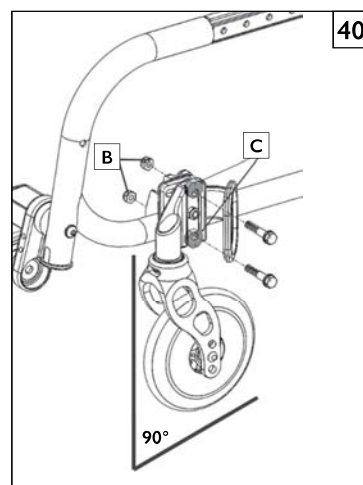**I. ANTI-TIP RECEIVERS** 41

Sunrise Medical recommends anti-tip tubes for all wheelchairs.

Use a torque setting of 360 in-lbs (40.1Nm) when setting up the anti-tip receivers (D).

NOTE— See section, *Rear axles and axle plates*, for more adjustment information.

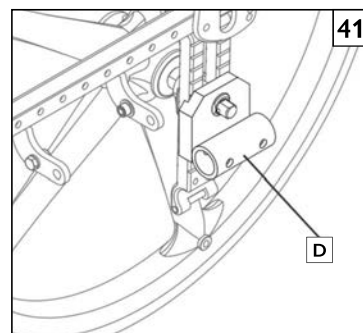

J. ARMREST RECEIVER ATTACHMENT 42 43



Mounting

1. Thread the two screws and washers (A) through the rear side frame tube, and into the single post height-adjustable armrest receiver (B).
2. Tighten the hardware to 120 in-lbs (13.6Nm).

Adjustment

1. To adjust the fit of the Single Post Armrest in the receiver, loosen the 4 hex bolts (C) by using a 7/16" wrench.
2. With the armrest assembly in the receiver (B), press firmly on the outside of the receiver.
3. Maintain pressure on the receiver and re-tighten two of the hex bolts (C).
4. Remove the armrest assembly and re-tighten the remaining two hex bolts.
5. The armrest should fit firmly into the receiver and lessen any noise that may result from vibration.

NOTE – Armrest Receiver may share hardware with wheel lock assembly if required.

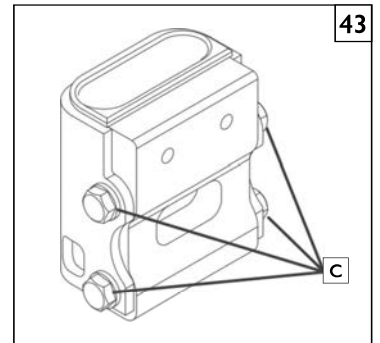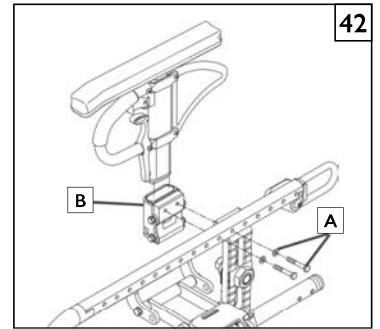

K. T-POST ARMREST 44

1. Lateral Adjustment

- a. Remove the receiver bolts (D).
- b. Move the receiver (E) forward or back to the desired position.
- c. Tighten the hardware to 120 in-lbs (13.6Nm).


2. Height Adjustment

- a. Remove the screws for the kids arm stop (F).
- b. Using one of the three preset holes in armrest post, adjust to the preferred height.
- c. Replace and tighten hardware. to 120 in-lbs (13.6Nm).

3. Tolerance Adjustment

- a. Tighten or loosen the set screw (G) as desired to lessen noise as a result of vibration.

NOTE – Armrest Receiver may share hardware with wheel lock assembly if required.

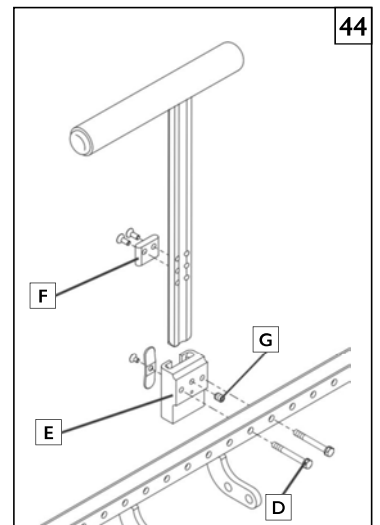

L. STANDARD FLIP-UP ARMREST 45

1. Height Adjustment


- a. Loosen set screws (H), and hex head bolts (I).
- b. Move armrest clamps (L) up or down backrest posts to desired position.
- c. Make sure that the set screws (H) are aligned with the adjustment holes (J) on the back cane (K).
- d. Thread the set screws so that they are flush with the clamp body, and hold the adjustment securely.

NOTE – Do not overtighten the set screws. There is a chance that they could fall inside the backcane.

- e. Tighten the hex head bolts to secure the armrest in the new position.

2. Angle Adjustment

- a. Loosen cam Bolt (L), and rotate the stop (M) to achieve the desired angle of the armrest.
- b. Tighten the cam bolt (L) to lock in the adjustment.

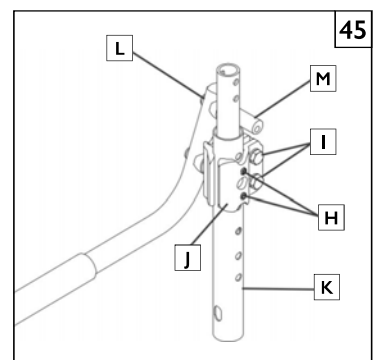

M. FLIP-UP ARMRESTS (ADJUSTABLE LOCKING, AND ADJUSTABLE LOCKING WITH ADJUSTABLE LENGTH) 46

1. Height Adjustment

- Loosen the clamp hardware (A).
- Move armrest clamps (B) up or down backrest posts to desired position.
- Make sure that the set screws (A) are aligned with the adjustment holes on the backrest.
- Thread the set screws so that they are flush with the clamp body, and hold the adjustment securely.

NOTE – Do not overtighten the set screws. There is a chance that they could fall inside the backrest.


- Tighten the clamp hardware (A) to secure the armrest in the new position.

2. Angle-Adjustment

- Loosen adjustment bolt (C) and the cam bolt (D).
- Lift the armrest to the desired position.
- Tighten cam bolt (D) to 120 in-lbs (13.6Nm).
- Tighten the angle adjustment bolt (C) to 45 in-lbs (5.1Nm).

3. Length-Adjustment (optional)

- Remove foam grip or armpad (E) from armrest.
- Loosen the nut and screw (F) in the adjustable flip-up tube.
- Reposition the arm tube at the desired length.
- Re-tighten the screw and nut (F).
- Re-attach foam grip or armpad back in place.

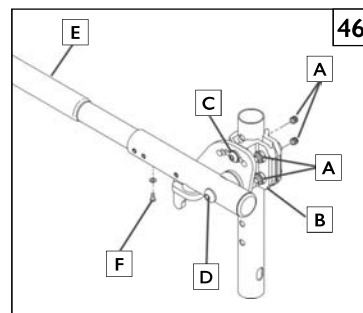

N. FOOTREST SYSTEM 47 48 49 50

The footrest position is key to keeping the body in the proper alignment, and providing a stable support for your legs and torso. Make sure that your Sunrise dealer has correctly adjusted your footrests and/or legrests with the advice of a healthcare professional. The original setup should not be changed without first checking with that advisor. Legrests and footrests should be swung out of the way, or removed for transfers.

NOTE – Footplate must have at least 2 inches (51mm) of clearance between the footplate and the ground to prevent hitting obstacles and risking a fall or tip-over.

1. Footrest/Footplate positioning using the rotational clamp

- Loosen the two rotational/angle clamp screws (G).
- Rotate the footrest/ footplate until the desired position and angle is achieved.
- Tighten the clamp hardware to proper torque (DO NOT EXCEED a 120 in-lb (13.6Nm) max torque).

2. Footrest positioning using footplate spacers





- Remove footplate spacer (A) from front or rear of pivot block (B).
- Slide footplate to desired depth position, fore or aft.
- Replace both footplate spacers to the front or rear of the pivot block.

3. Height range adjustment (Direct Mount Footrest)

- Adjust the footplate mounting position by removing the button head screw from the adjustment hole (H) and moving the assembly to the desired position.
- Tighten hardware to proper torque (DO NOT EXCEED a 120 in-lb (13.6Nm) max torque).


4. Height range adjustment (Extension Mount Footrest)

- Loosen set screw (M).
- Slide footrest extension tube up or down inside frame tube to desired height.
- Tighten set screw to proper torque (DO NOT EXCEED a 120 in-lb (13.6Nm) max torque).

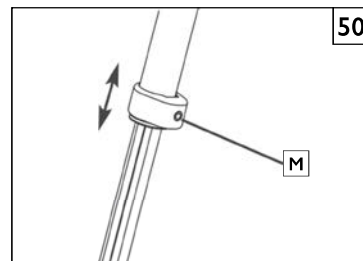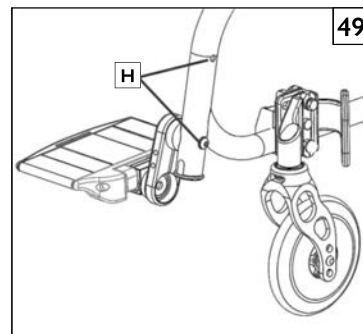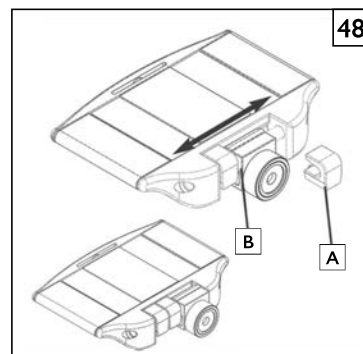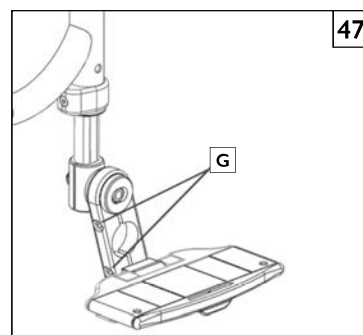


5. **Aluminum Angle Adjustable Footplate** 51


- Loosen bolts (I).
- Adjust footplate (J) to desired angular position.
- Re-tighten hardware (I).

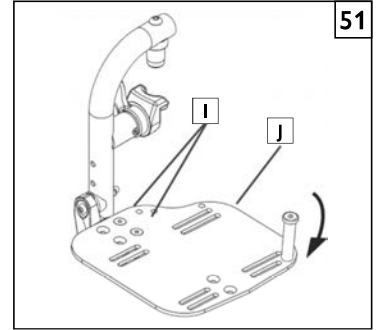**O. ANGLE ADJUSTABLE BACKREST**1. **Backrest Height Adjustment** 52

- You will see the Backrest Height Adjust hardware on the inside of the frame (A). Loosen and remove from both sides of the frame.
- Adjust the backtube (B) to the desired backrest height. (measured with chair unfolded, from top of seat sling to highest point on upholstery) and align threaded insert of back cane with the closest hole in frame.
- Insert bolt through frame and thread into the insert in back cane.
- Torque fastener (A) on both sides of chair to 50 in-lbs (5.7 Nm).

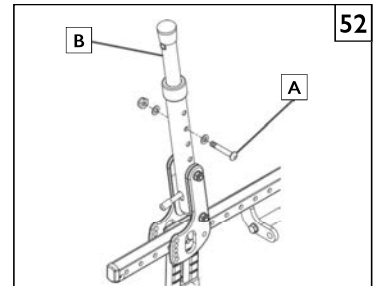2. **Angle Adjustment** 53

- Loosen remove the button head screws (D) and hardware (C).
- Adjust backrest to desired angle.
- Attach the hardware (D and C) into new adjustment hole, and tighten button head screws. Use a Torque of 120 in-lbs (13.6 Nm) for screw (D).
- Repeat for opposite side.

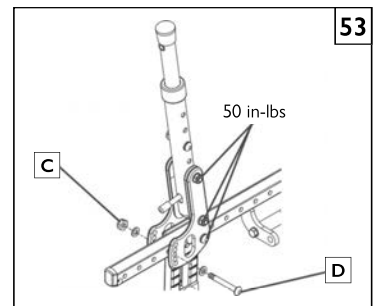3. **Back Depth Adjustment** 54


NOTE – This adjustment is intended to compensate for differences in after-market backrest thickness and/or contour. The back canes can be adjusted fore and aft relative to the seat so that the backrest support surface does not change the location of the user, regardless of the backrest mounting location. This ensures that the center of gravity of the user relative to the axle location, is not altered due to after-market backrest thickness or contour.

NOTE – Sunrise has no recommendations for Depth Adjustable Backrest adjustments and how they might affect transit situations.

When adding an after-market back, the back canes can be moved forward or rearward by removing hardware (E and F) and repositioning the backrest pivot plate (G) in the pre-drilled holes on the frame.


Tighten Screws (E and F) to 120 in-lbs (13.6 Nm).

NOTE – In most cases the axle plate should move with the backrest bracket and back canes as the adjustment is made.

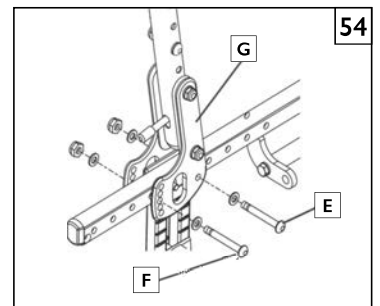

P. XLOCK™ TECHNOLOGY 55

1. **Frame Width Adjustment either 1" (25mm) (only adjust 1 side) or 2" (51mm) of width (adjust both sides).**
 - a. Remove the Hex head screws, and washers (H) from the left and/or right front side frame tabs (I) depending if you want a 1" or 2" adjustment (25 or 51mm).
 - b. Re-align the XLOCK assembly with the correct adjustment holes.
 - c. Thread the hex head screws (H) and washers through the tab holes and into the X-Lock brace.
 - d. Tighten the hex head screws to 120 in-lbs (13.6 Nm).

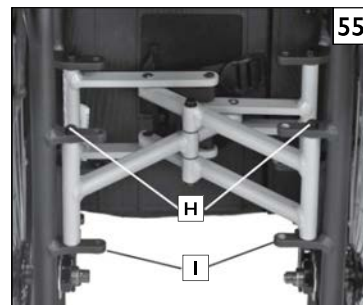

Q. DYNAMIC BACKREST 56 57



1. **Dynamic Backrest Elastomer Replacement.**
 - a. Remove socket head screw (J) and lock nut (K).
 - b. Using a flat head screw driver, gently pry out the elastomer (L) as shown.
 - c. Firmly press the new desired elastomer into place and align holes in elastomer with holes in plate (M).
 - d. Replace and tighten screws removed above, the nylock nut (K) needs to be fully engaged.



WARNING

If the chair is equipped with the Dynamic Backrest option, the lockout feature must be in the locked position on both push handles prior to any type of transport of the chair.


2. **Dynamic Backrest Lock Engagement.**
 - a. Pull key ring (A) and swing lock downward to unlock backrest.
 - b. Swing lock upward to lock the backrest.

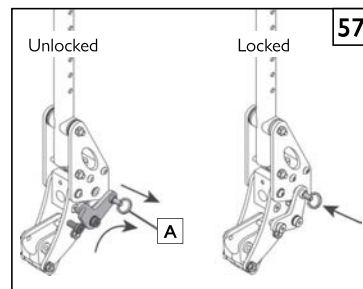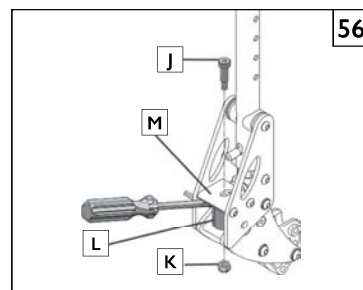

R. SIDEGUARD WITH T-POST ARMREST 58


1. **Installation of sideguard.**
 - a. Position the Sideguard (B) and Sideguard clamp (C) onto the T-post at a height that will locate the bottom edge of the sideguard next to the frame.
 - b. Insert two bolts (D) with washer and tighten using 3/16 inch hex key.
 - c. Your sideguard and T-post armrest can now be inserted into the receiver.

NOTE – After installing receiver hardware and inserting the side guard, check for interference. Don't operate the wheelchair if the sideguard interferes with any of the other components.

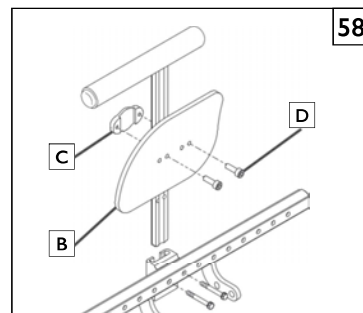


S. BACKREST TENSION ADJUSTABLE 59 60 61**1. To install the Backrest Tension Adjustable**

- Slide Velcro straps (E) over the backrest frame (F) section. Make sure to include at least one strap below the towel bar (if using a rigid chair).
- Tighten the straps appropriately to desired tension level. Straps should be installed when chair is unfolded. **DO NOT** overtighten straps as this will cause undue strain upon the chair frame. The difference in width between the top and bottom of the backrest should not exceed $\pm 0.5"$ ($\pm 13\text{mm}$).
- If using integral push handles (G), slide straps from bottom of backrest upward.
- Install backrest cover at desired level and fold over rear of Velcro strapping system (H). The Zippie patch should be upright on the rear of the chair.
- Finish installation by placing vanity flap (center panel) down onto Velcro on the seat sling to secure attachment (I).

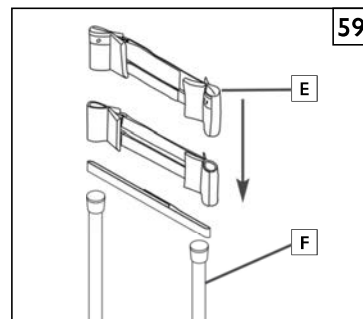
**2. Adjusting the Backrest Tension Adjustable**

Suggest using anti tips while making any adjustments. Ensure anti-tips are safely secured and in a position to prevent the wheelchair from tipping backwards.

- User can transfer into wheelchair. Place wheel locks in the locked position.
- From the rear of the wheelchair the attendant can lift the Vanity Flap (center panel) to access the strap system. Adjust straps for optimal balance and trunk alignment. Ensure the Velcro straps have a minimum of 2 inches (51mm) of engagement, hook securing to loop. Press the Velcro together to ensure it's securely engaged.
- Once adjustments have been finalized replaced vanity flap to its original position.

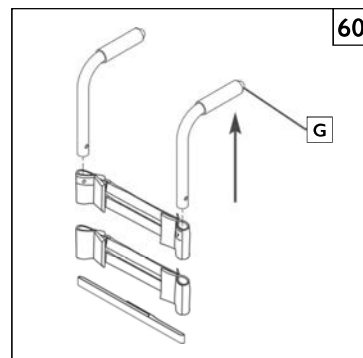
 WARNING

Any changes made to the straps will affect the center of gravity. Suggest the user have the attendant stationed behind the wheelchair to prevent the wheelchair from tipping backwards while they become accustomed to the adjustment.

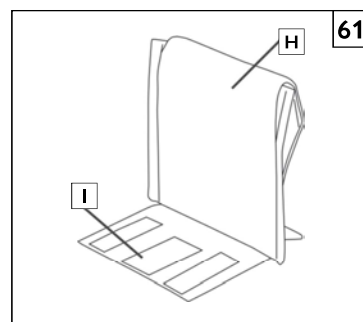

A. FOR LIFETIME

Frame and cross-brace (if applicable) warranty:

1. Although the anticipated useful service time of this wheelchair is five years, Sunrise guarantees the frame and cross brace against defects in material and workmanship for life or for as long as the original purchaser owns the chair.
2. This warranty does not apply if:
 - a. The chair is subject to abuse.
 - b. The chair is not maintained as recommended in the owner's manual.
3. The chair is transferred to a different person from the original owner.

B. FOR ONE (1) YEAR

We warrant all Sunrise-made parts and components of this wheelchair against defects in materials and workmanship for one year from the date of first consumer purchase. An invoice, as proof of purchase may be required.

Backrest Tension Adjustable (Balistic & 3DX Vented)

Each Backrest Tension Adjustable is carefully inspected and tested to provide peak performance. Every Backrest Tension Adjustable is guaranteed to be free from defects in materials and workmanship for a period of twelve (12) months from the date of purchase provided normal use. Should a defect in materials or workmanship occur within twelve months from the original date of purchase, Sunrise Medical will, at its option, repair or replace it without charge. This warranty does not apply to puncture, tears or burns. Claims and repairs should be processed through the nearest authorized dealer. Except for express warranties made herein, all other warranties including implied warranties of merchantability and warranties of fitness for particular purpose are excluded. There are not warranties which extend beyond the description of the face hereof. Remedies for breach of express warranties herein are limited to repair or replacement of the goods. In no event shall damages for breach of any warranty include any consequential damages or exceed the cost of non-conforming goods sold.

C. LIMITATIONS

1. We do not warrant:
 - a. Tires and tubes, upholstery, pads and push-handle grips.
 - b. Damage from neglect, accident, misuse, or from improper installation or repair.
 - c. Products modified without Sunrise Medical's express written consent.
 - d. Damage from exceeding the weight limit.
2. This warranty is VOID if the original chair serial number tag is removed or altered.
3. This warranty applies in the USA and CANADA only. Check with your dealer to find out if international warranties apply.
4. This warranty is not transferable and only applies to the first consumer purchase of this wheelchair through an authorized Sunrise Medical dealer.

D. WHAT WE WILL DO

Our sole liability is to repair or replace covered parts. This is the exclusive remedy for consequential damages.

E. WHAT AUTHORIZED DEALER MUST DO

Obtain from Sunrise Medical, while this warranty is in effect, prior approval for return or repair of covered parts. Contact Customer Service for a Returned Material Authorization (RMA) number and information as to where to return the product. Upon contacting Customer Service please provide Model number, Serial number, description of what is required for service/repair, and any additional information as to reason for service being performed to the wheelchair.

F. NOTICE TO CONSUMER

1. You must pay the cost of labor to repair, remove or install parts even if they are covered under warranty.
2. If allowed by law, this warranty is in place of any other warranty (written or oral, express or implied, including a warranty of merchantability, or fitness for a particular purpose).
3. This warranty gives you certain legal rights. You may also have other rights that vary from state to state or province to province.

G. ADDITIONAL WARRANTY INFORMATION

For goods provided by Sunrise Medical Pty Ltd in Australia, our goods come with a guarantee by Sunrise that cannot be excluded under the Australian Consumer Law. You are entitled to a replacement or refund for a major failure and for compensation for any other reasonably foreseeable loss or damage. You are also entitled to have the goods repaired or replaced if the goods fail to be of acceptable quality and the failure does not amount to a major failure. The benefits to you given by this warranty are in addition to your other rights and remedies under a law in relation to the goods to which the warranty relates.

Record your serial number here for future reference:



A series of horizontal lines for writing notes, spanning the width of the page below the pen illustration.



A series of horizontal lines for writing notes, spanning the width of the page below the pen illustration.

Sunrise Medical S.r.l.
Via Riva, 20 – Montale
29122 Piacenza
Italia
Tel.: +39 0523 573111
www.SunriseMedical.it

Sunrise Medical AG
Erlenauweg 17
CH-3110 Münsingen
Schweiz/Suisse/Svizzera
Tel +41 (0)31 958 3838
www.SunriseMedical.ch

Sunrise Medical AS
Delitoppen 3
1540 Vestby
Norge
Telefon: +47 66 96 38 00
post@sunrisemedical.no
www.SunriseMedical.no

Sunrise Medical AB
Neogatan 5
431 53 Mölndal
Sweden
Tel.: +46 (0)31 748 37 00
post@sunrisemedical.se
www.SunriseMedical.se

MEDICCO s.r.o.
H – Park, Heršpická 1013/11d,
639 00 Brno
Czech Republic
Tel.: (+420) 547 250 955
Fax: (+420) 547 250 956
www.medicco.cz
info@medicco.cz
Bezplatná linka 800 900 809

Sunrise Medical Aps
Mårkærvej 5-9
2630 Taastrup
Denmark
+45 70 22 43 49
info@sunrisemedical.dk
www.SunriseMedical.dk

Sunrise Medical Australia
11 Daniel Street
Wetherill Park NSW 2164
Australia
Ph: +61 2 9678 6600
Email: enquiries@sunrisemedical.com.au
www.SunriseMedical.com.au

Sunrise Medical (US) LLC
North American Headquarters
12002 Volunteer Blvd.
Mount Juliet, TN 37122, USA
(800) 333-4000
(800) 300-7502
www.SunriseMedical.com



© 2025 Sunrise Medical (US) LLC
MK-100090 Rev. E

Sunrise Medical GmbH
Kahlbachring 2-4
D-69254 Malsch
Deutschland
Tel.: +49 (0) 7253/980-0
Fax: +49 (0) 7253/980-222
www.SunriseMedical.de

Sunrise Medical Ltd.
Thorns Road
Brierley Hill
West Midlands
DY5 2LD
England
Phone: 0845 605 66 88
Fax: 0845 605 66 89
www.SunriseMedical.co.uk

Sunrise Medical S.L.
Polígono Bakiola, 41
48498 Arrankudiaga – Vizcaya
España
Tel.: +34 (0) 902142434
Fax: +34 (0) 946481575
www.SunriseMedical.es

Sunrise Medical Poland
Sp. z o.o.
ul. Elektronowa 6,
94-103 Łódź
Polska
Telefon: + 48 42 275 83 38
Fax: + 48 42 209 35 23
E-mail: pl@sunrisemedical.de
www.Sunrise-Medical.pl

Sunrise Medical B.V.
Defensiedok 20
3433 NE Nieuwegein
The Netherlands
T: +31 (0)30 – 60 82 100
F: +31 (0)30 – 60 55 880
E: info@sunrisemedical.nl
www.SunriseMedical.nl

Sunrise Medical HCM B.V.
Vossenbeemd 104
5705 CL Helmond
The Netherlands
T: +31 (0)492 593 888
E: customerservice@sunrisemedical.nl
www.SunriseMedical.nl
www.SunriseMedical.eu (International)

Sunrise Medical S.A.S
ZAC de la Vrillonnerie
17 Rue Mickaël Faraday
37170 Chambray-Lès-Tours
Tel : + 33 (0) 2 47 55 44 00
Email: info@sunrisemedical.fr
www.SunriseMedical.fr

Sunrise Medical Canada Inc.
1000 Creditstone Rd., Unit #2
Concord, ON, L4K 4P8
Canada
Phone: 1-800-263-3390
Fax: 1-800-561-5834
www.SunriseMedical.ca